

Dräger X-am[®] 5000

approved as type MQG 0010

Multi-Gas Monitor
Technical Manual



Content

For Your Safety	4
Intended Use	4
Tests and Approvals	5
Intended operating area and operating conditions	6
Safety instructions	6
What is What	8
Front panel	8
Rear panel	8
Display	8
Special symbols	9
Configuration	10
Standard gas configuration	10
Standard device configuration	12
Operation	13
Preparations for operation	13
Switching on the device	13
Switching off the device	14
Before entering the workplace	14
During operation	16
Calling the Info Mode	17
Calling the Info-Off Mode	17
Calling the Quick Menu	18
Possible functions of the quick menu	18
Quick menu "Delete peak values"	19
Calling the Calibration Menu	20
Calibration menu functions	20
Identifying Alarms	21
Concentration pre-alarm A1	21
Concentration main alarm A2	21
STEL / TWA exposure alarm	22
Battery pre-alarm	22
Battery main alarm	22
Device alarm	22
Operation with pump	23
Configuring the Device	26
Device settings	27
Read Database and Display Graphically	29
Faults, Cause and Remedy	30
Warning messages	30

Fault messages	33
Maintenance	38
Maintenance intervals	38
ToxicTwins	39
CO H ₂ compensation	39
Carry out manual bump test	40
Manual implementation without the documentation of results in the device memory	40
Menu implementation with the documentation of results in the device memory	41
Automatic implementation with the Bump Test Station	43
Calibrating the Device	45
Carrying out the fresh air calibration	46
Carrying out 1-button calibration	49
Calibrating the sensitivity for an individual measuring channel	51
Span calibration for CatEx	52
Replacing the batteries / rechargeable batteries	55
Charging the rechargeable batteries	56
Charging with the multiple charging station	56
Charging with charging module and plug-in power pack or vehicle charging adapter	58
Replacing the Sensors	59
Sensor warm-up acceleration	61
Cleaning	62
Storage	63
Disposal	63
Technical Data	64
X-am 5000	64
Order List	65
Accessories	66
Spare parts	68

For Your Safety

General safety statements

- Before using this product, carefully read the associated Instructions for Use. This document does not replace the Instructions for Use.

Definitions of alert icons

The following alert icons are used in this document to provide and highlight areas of the associated text that require a greater awareness by the user. A definition of the meaning of each icon is as follows:

DANGER

Indicates an imminently hazardous situation which, if not avoided, will result in death or serious injury.

WARNING

Indicates a potentially hazardous situation which, if not avoided, could result in death or serious injury.

CAUTION

Indicates a potentially hazardous situation which, if not avoided, could result in physical injury, or damage to the product or environment. It may also be used to alert against unsafe practices.

NOTICE

Indicates additional information on how to use the product.

Intended Use

Portable gas detection instrument for the continuous monitoring of the concentration of several gases in the ambient air within the working area and in explosion-hazard areas.

X-am 5000, depending on the device type and configuration of DrägerSensors: independent measurement of one up to five gases.

Tests and Approvals

Copies of the name plate and the declaration of conformity are provided in the enclosed supplementary documentation (order no. 90 33 890).

The BVS 10 ATEX E 080 X technical suitability test is based on the adjustment with the target gas.

Do not stick anything on the name plate on the gas detector.

The technical suitability tests are valid for the X-am 5000 gas detector and the calibration cradle. The explosion-protection approvals are only valid for the X-am 5000 gas detector; the calibration cradle must not be used in the Ex zone.

Intended operating area and operating conditions

Areas subject to explosion hazards, classified by zones

The instrument is intended for the use in explosion-hazard areas of Zone 0, Zone 1 or Zone 2 or in mines at risk due to fire damp. It is intended for use within a temperature range of -20 °C to +50 °C, and for areas in which gases of explosion groups IIA, IIB or IIC and temperature class T3 or T4 (depending on the batteries and rechargeable battery) may be present. If used in mines, the instrument is only to be used in areas known to have a low risk of mechanical impact.

Areas subject to explosion hazards, classified by divisions.

The instrument is intended for use in explosion-hazard areas according to Class I&II, Div. 1 or Div. 2 within a temperature range of -20 °C to +50 °C, and for areas where gases or dusts of groups A, B, C, D, E, F, G and temperature class T3 or T4 may be present (depending on the rechargeable battery and batteries).

WARNING:

CSA requirement: The sensitivity must be tested on a daily basis before first use with a known concentration of the gas to be measured in accordance with 25 to 50 % of the concentration limit value. The accuracy must be 0 to +20 % of the actual value. The accuracy can be corrected via calibration.

Safety instructions

WARNING

To reduce the danger of explosion, do not mix new batteries with old batteries and do not mix batteries made by different manufacturers.

WARNING

Always disconnect the device from the power pack before carrying out any maintenance operations.

WARNING

Substitution of components may impair intrinsic safety.

CAUTION

Not tested in an oxygen-enriched atmosphere (>21 % O₂).

WARNING

High off-scale readings may indicate an explosive concentration.

▲ CAUTION

Use only supply units ABT 0100 (83 22 237), HBT 0000 (83 18 704) or HBT 0100 (83 22 244). Check the supply unit for approved batteries and applicable temperature class.

Note the following for CSA (Canadian Standards Association) applications:

For the CSA approval only the functions of the device component that is used to measure flammable gases are tested. The device is not approved by CSA for use in mining.

▲ WARNING:

Before daily use, test the sensitivity with a known concentration of the applicable gas corresponding to 25 to 50% of the maximum concentration. The accuracy must be within a range of 0 to +20% of the actual value. Perform a calibration to correct the accuracy if necessary.

Only applies for class II certification. CSA standard C22.2 no. 152 does not contain any requirements for class II hazard areas. Therefore this device was not tested for class II by the CSA. The sensor may become blocked and not measure the gas correctly or not warn the user that gas measurement is not possible.

▲ WARNING

CSA requirement: Measured values over the full scale value are displayed as an explosive concentration.


NOTICE

CSA requirement: a measurement suitability test must be conducted for flammable gases.

What is What

Front panel


- 1 Gas entry
- 2 Alarm LED
- 3 Buzzer
- 4  key
- 5  key
- 6 Display
- 7 Tool for replacing the sensor

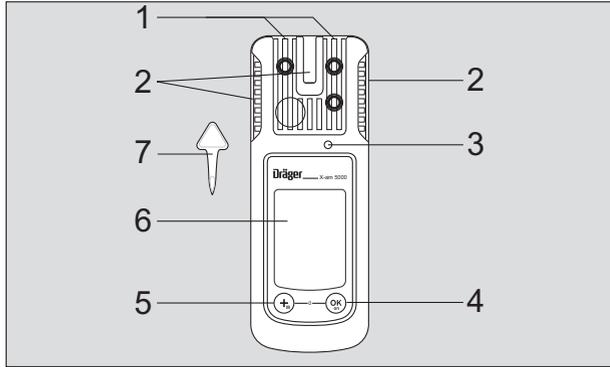

00223999_02.eps

Rear panel

- 1 IR interface
- 2 Fastening clip
- 3 Type plate
- 4 Charging contacts
- 5 Power pack
- 6 Serial no.

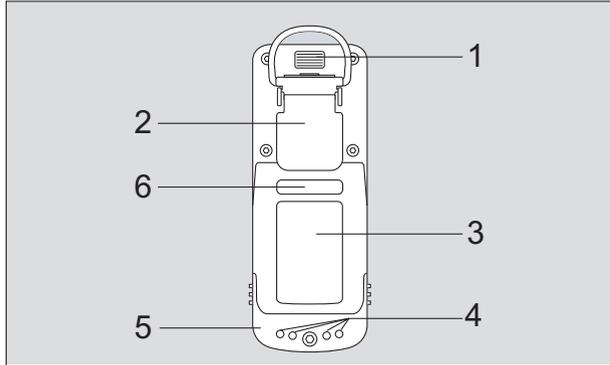

00223999_02.eps


Display

for 5 measuring channels only:

- 1 Measured gas display with unit
- 2 Measured value display
- 3 Special symbols

other:

- 4 Measured gas display
- 5 Measured gas display with unit
- 6 Special symbols

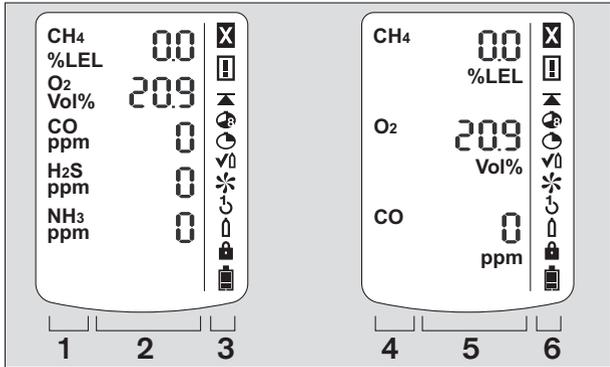

00223999_02_en.eps

The following only shows the device version with 5 measuring channels.

Special symbols

-  Fault message, refer to page 17
-  Warning message, refer to page 17
-  The peak value display for all measuring gases, refer to page 17
-  The exposure evaluation display (TWA) for measuring gases, e.g., H₂S and CO, refer to page 17
-  The exposure evaluation display (STEL) for measuring gases, e.g., H₂S and CO, refer to page 17
-  The device is set to function test with gas (bump test), refer to page 40
-  The device is set to the fresh air calibration function, refer to page 46
-  The device is set to the 1-button calibration function, refer to page 47
-  The device is set to the single gas calibration function, refer to page 50
-  The function for password entry is active, refer to page 20
-  Battery / rechargeable battery 100 % full
-  Battery / rechargeable battery 2/3 full
-  Battery / rechargeable battery 1/3 full
-  Battery / rechargeable battery empty

Marking offset channels:

Feature	Reading on the display
ToxicTwins	HCN+
CO H ₂ compensation	CO+

Configuration

Standard gas configuration

DrägerSensor	Measuring range ¹⁾	Alarm A1 ¹⁾			Alarm A2 ¹⁾		
		setpoint	can be acknowledged	self-latching	setpoint	can be acknowledged	self-latching
CatEx 125 PR [%LEL]	0 to 100	20	Yes	No	40	No	Yes
CatEx 125 PR Gas [%LEL]	0 to 100	20	Yes	No	40	No	Yes
XXS O ₂ [vol. %]	0 to 25	19 ²⁾	No	Yes	23	No	Yes
XXS O ₂ 100 [vol. %]	0 to 100	18.5 ²⁾	No	Yes	24	No	Yes
XXS O ₂ LS / CO-LC [vol. %], [ppm]	0 to 25 O ₂ 0 to 2000 CO	19 O ₂ 30 CO	No Yes	Yes No	23 O ₂ 60 CO	No No	Yes Yes
XXS O ₂ / H ₂ S-LC [Vol%], [ppm]	0 to 25 O ₂ 0 to 100 H ₂ S	19 O ₂ 5 H ₂ S	No Yes	Yes No	23 O ₂ 10 H ₂ S	No No	Yes Yes
XXS CO [ppm]	0 to 2,000	30	Yes	No	60	No	Yes
XXS CO LC [ppm]	0 to 2,000	30	Yes	No	60	No	Yes
XXS CO-LC/H ₂ S-LC [ppm]	0 to 2,000 0 to 100	30 5	Yes Yes	No No	60 10	No No	Yes Yes
XXS CO-LC/O ₂ [ppm], [vol.-%]	0 to 2,000 CO 0 to 25 O ₂	30 CO 19 O ₂	Yes No	No Yes	60 CO 23 O ₂	No No	Yes Yes
XXS CO HC [ppm]	0 to 10,000	600	Yes	No	1,200	No	Yes
XXS CO H ₂ -CP [ppm]	0 to 2.000	30	Yes	No	60	No	Yes
XXS H ₂ [ppm]	0 to 2.000	200	Yes	No	400	No	Yes
XXS H ₂ S [ppm]	0 to 200	5	Yes	No	10	No	Yes
XXS H ₂ S LC [ppm]	0 to 100	5	Yes	No	10	No	Yes
XXS H ₂ S HC [ppm]	0 to 1,000	10	Yes	No	20	No	Yes
XXS H ₂ S/CO [ppm]	0 to 200 H ₂ S 0 to 2,000 CO	5 H ₂ S 30 CO	Yes	No	10 H ₂ S 60 CO	No	Yes
XXS H ₂ S-LC / CO-LC [ppm]	0 to 100 H ₂ S 0 to 2000 CO	5 H ₂ S 30 CO	Yes Yes	No No	10 H ₂ S 60 CO	No No	Yes Yes
XXS NO [ppm]	0 to 200	25	Yes	No	50	No	Yes
XXS NO ₂ [ppm]	0 to 50	5	Yes	No	10	No	Yes
XXS SO ₂ [ppm]	0 to 100	0,5	Yes	No	1	No	Yes
XXS PH ₃ [ppm]	0 to 20	0.1	Yes	No	0.2	No	Yes
XXS PH ₃ HC [ppm]	0 to 2,000	5	Yes	No	10	No	Yes
XXS HCN [ppm]	0 to 50	1.9	Yes	No	3.8	No	Yes
XXS HCN PC [ppm]	0 to 50	5	Yes	No	10	No	Yes
XXS NH ₃ [ppm]	0 to 300	20	Yes	No	40	No	Yes
XXS CO ₂ [vol. %]	0 to 5	0.5	Yes	No	1	No	Yes
XXS Cl ₂ [ppm]	0 to 20	0.5	Yes	No	1	No	Yes
XXS H ₂ HC [vol. %]	0 to 4	0.8	Yes	No	1.6	No	Yes

DrägerSensor	Measuring range ¹⁾	Alarm A1 ¹⁾			Alarm A2 ¹⁾		
		setpoint	can be acknowledged	self-latching	setpoint	can be acknowledged	self-latching
XXS OV [ppm]	0 to 200	10	Yes	No	20	No	Yes
XXS OV A [ppm]	0 to 200	10	Yes	No	20	No	Yes
XXS Odorant [ppm]	0 to 40	10	Yes	No	20	No	Yes
XXS Amine [ppm]	0 to 100	10	Yes	No	20	No	Yes
XXS COCl ₂ [ppm]	0 to 10	0.1	Yes	No	0.2	No	Yes
XXS O ₃ [ppm]	0 to 10	0.1	Yes	No	0.2	No	Yes
XXS NO ₂ LC [ppm]	0 to 50	0,5	Yes	No	1,0	No	Yes

- 1) Different settings can be selected to meet customer requirements on delivery. The current setting can be checked and changed with the Dräger CC Vision software. A version of Dräger CC-Vision suitable for the Dräger X-am 5000/2000 can be downloaded on the product page of the X-am 5000: www.draeger.com.
- 2) In the case of O₂ A1 is the lower alarm setpoint: an alarm is issued if the value is too low.

Standard device configuration

NOTICE	
Only trained personnel are permitted to make changes to the device configuration.	
Dräger X-am[®] 5000¹⁾	
Bump test mode ²⁾	Extended bump test
Fresh air calibration ²⁾	ON
Operating signal ^{2) 3)}	ON
Capture range	ON
Switch off ²⁾	allowed
LEL factor ²⁾ (ch ₄)	4.4 (vol. %) (4.4 vol. % corresponds to 100 %LEL)
STEL ^{2) 4) 5)} (short-term average)	STEL function - disabled Average value duration = 15 minutes
TWA ^{2) 5) 6)} (shift average)	TWA function - disabled Average value duration = 8 hours
Alarm A1 ⁷⁾	can be acknowledged, non-latching, pre-alarm, rising flank
Alarm A1 at O ₂ sensor ⁷⁾	cannot be acknowledged, latching, like main alarm, falling flank
Alarm A2 ⁷⁾	cannot be acknowledged, latching, main alarm, rising flank

- 1) X-am[®] is a registered trademark of Dräger.
- 2) Different settings can be selected to meet customer requirements on delivery. The current setting can be checked and changed with the Dräger CC Vision software.
- 3) A periodic short signal indicates the operating capacity of the instrument. If there is no operating signal, correct operation cannot be guaranteed.
- 4) STEL: average value of an exposure over a short period, generally 15 minutes.
- 5) Interpretation only if the sensor is designed for this.
- 6) TWA: shift averages are workplace limit values for generally eight hours per day of exposure for five days a week during a working life.
- 7) Latching and acknowledgement of alarms A1 and A2 can be configured with the Dräger CC Vision PC software.

Changing the standard configuration: See “Configuring the Device” on page 26.

 WARNING
After a basic initialization has been carried out with the PC software Dräger CC Vision, individual alarm settings may have been changed.

Selecting or disabling the capture ranges (only applies for the measuring mode):

The capture range is selected in the measuring mode (factory setting) and permanently disabled in calibration mode.

The CC-Vision PC software can be used to select or disable the capture ranges for the measuring mode.

Operation

Preparations for operation

- Before using the instrument for the first time, insert a charged NiMH T4 power pack or batteries approved by Dräger, see "Changing the batteries" on page 55.
- The instrument is now ready for operation.

▲ WARNING
<p>To reduce the risk of ignition of a flammable or explosive atmosphere, strictly adhere to the following warning statements:</p> <p>Only use power pack types ABT 01xx, HBT 00xx or HBT 01xx. See the marking on the rechargeable battery for permitted rechargeable batteries and the corresponding temperature class.</p> <p>Substitution of components may impair intrinsic safety.</p>

Switching on the device

- Press and hold the  key for approx. 3 seconds until the countdown » **3 . 2 . 1** « shown in the display has elapsed.
 - All the display segments, including the visual, audible and vibration alarms, are activated for a short time.
 - The software version is displayed.
 - The device performs a self test.
 - The next sensor which is next due for calibration is displayed with the days remaining until the next calibration, e.g., » **Ex %LEL CAL 20** «.
 - The time until the bump test interval elapses is displayed in days, e.g., » **bt 123** «.
 - All A1 and A2 alarm thresholds and »  « (TWA)¹⁾ and »  « (STEL)¹⁾ for all toxic gases (e. g. H₂S or CO) are displayed consecutively.
 - During the sensor warm-up phase:
 - The display for the measured value flashes
 - The special symbol »  « is displayed.
 - No alarms are issued during the warm-up phase.
 - The red LEDs flash.
 - The gas detector is ready to measure when the measured values no longer flash and the red LEDs are no longer illuminated. The special symbol »  « may continue to be displayed if corresponding warnings (e.g. not yet ready for calibration) are active (to view the warnings, see the technical manual).
- Press the  key to cancel the display of the activation sequence.

1) Only when activated in the instrument configuration. Delivery condition: not activated.

Switching off the device

- Press and hold the  key and  key at the same time until the countdown » 3 . 2 . 1 « shown in the display has elapsed.

Before the device is switched off, the visual, audible and vibration alarms are activated for a short time.

Before entering the workplace

WARNING

Before any measurements relevant to safety are made, check the adjustment with a bump test, adjust if necessary and check all alarm elements. If national regulations apply, a bump test must be performed according to the national regulations. Faulty adjustment may result in incorrect measuring results, with possible serious consequences.

WARNING

In an oxygen enriched atmosphere (>21 vol. % O₂), the explosion protection cannot be guaranteed; remove instrument from the explosion-hazard area.

CAUTION

The CatEx sensor is intended for measurements of flammable gases and vapours mixed with air (i.e. O₂ content ≈ 21 vol.%). Incorrect measured values may be displayed in the case of oxygen deficient or oxygen enriched environments.

NOTICE

If the gas detector is used for offshore applications, a distance of 5 m to a compass must be complied with.

- Switch on the device. The current measured values are shown in the display.
- Observe any warning »  « or fault messages »  «.
 -  The device can be operated normally. If the warning message does not go out automatically during operation, the device must be maintained after the end of use.
 -  The device is not ready to measure and requires maintenance.
- If one of these special symbols is displayed, appropriate measures, refer to page 30 to page 33, must be taken.

- Check that the gas inlet opening on the device is not covered.

⚠ WARNING

Explosion hazard! To reduce the risk of flammable or explosive atmospheres igniting, it is essential that the warning notices below are observed:

- Fractions of catalytic poisons in the measuring gas (e.g. volatile silicon, sulphur, heavy metal compounds or halogenated hydrocarbon) can damage the Cat Ex sensor. If the CatEx sensor can no longer be calibrated to the target concentration, the sensor must be replaced.
- In case of measurements in oxygen-deficient atmosphere (<12 vol. % O₂) the CatEx sensor may show incorrect displays; in this case, a reliable measurement with a CatEx sensor is not possible.
- In an oxygen enriched atmosphere (>21 vol. % O₂), the explosion protection cannot be guaranteed; remove instrument from the Ex area.
- High values outside the display area indicate an explosive concentration where applicable.

During operation

- During operation, the measured values for every measured gas are displayed.
- In the event of an alarm, the corresponding displays, the visual, audible and vibration alarms are activated – see chapter “Identifying Alarms”.
- If a measuring range is exceeded or a negative drift occurs, the following displays are shown instead of the measured value display:
 - »  « (concentration too high) or
 - »  « (measuring range not reached) or
 - »  « (blocking alarm).
- If an O2 sensor is fitted and this sensor measures an O2 concentration of below 12 vol. %, an error is indicated with » - - « on the ex-channel instead of a measured value if the measured value is below the pre-alarm threshold (not with the setting CH4 with measuring range >100 %LEL).
- After the measuring range of the TOX measuring channels has been exceeded temporarily (up to one hour), checking the measuring channels is not necessary.

In the event of an alarm, the corresponding displays, including the visual, audible and vibration alarms, are activated – see “Identifying Alarms” on page 21.

NOTICE

Special states in which there is no measuring operation (quick menu, calibration menu, warm-up of sensors, password input) are indicated by a visual signal (slow flashing of the alarm LED ).

If the measuring range is exceeded significantly on the CatEx channel (very high concentration of flammable materials), a blocking alarm is triggered. This CatEx blocking alarm can be acknowledged manually by switching the device off and back on again in fresh air.

In configuration setting CH₄ with measuring range 100 vol. %, no blocking alarm is triggered as the heat conductance measurement principle is used.

⚠ CAUTION

The measuring range 0 to 100 vol. % CH₄ is not suitable for monitoring explosive mixtures in the measuring range from 0 to 100%LEL.

⚠ WARNING

If the DrägerSensor CatEx 125 PR is used in the gas detector, a zero point and sensitivity calibration must be carried out after experiencing an impact load that results in a non-zero display when exposed to fresh air. This warning does not apply if the DrägerSensor CatEx 125 PR Gas is used.

Calling the Info Mode

- In measuring mode, press the  key for approx. 3 seconds.

If any warning or fault messages exist, the corresponding information or error codes are displayed (page 30 to page 37).

Press the  key successively for the next display.

The peak values and the exposition values TWA¹⁾ and STEL¹⁾ are displayed.

 Warning messages are displayed. Numerical codes of warning messages: see page 30.

 key

 Fault messages are displayed. Numerical codes of fault messages: see page 33.

 key

 The peak values = the maximum measured values in the case of, e.g., CO, H₂S, ... or the minimum measured values in the case of O₂ within the storage interval are displayed

 key

 The average values of the exposures based on a shift of, e.g., 8 hours (TWA) of all the active sensors for the exposure evaluation are displayed

 key

 The short-term values (STEL) = average values of the concentrations over the average value duration of all the active sensors for the exposure evaluation are displayed

 key

The device is in measuring mode again

- If no key is pressed for 10 seconds, the device returns automatically to measuring mode.

Calling the Info-Off Mode

When the device is in a deactivated state, press the  key.

The name of the gas, measuring unit and measuring range limit value are displayed for all channels.

Pressing the  key again exits the Info Off mode (or via timeout).

1) Only when activated in the device configuration. Delivery status: not activated.

Calling the Quick Menu

- Only the fresh air calibration is activated in the quick menu on delivery. The PC software Dräger CC Vision can be used to activate the bump test for the quick menu and/or the function for displaying and deleting peak values.
- In measuring mode, press the \oplus key three times.
If no functions have been activated in the quick menu, the device remains in measuring mode.
- You can select the activated functions of the quick menu by pressing the \oplus key.
- Press the $\textcircled{\text{OK}}$ key to call the selected function.


Possible functions of the quick menu

-  Bump test, refer to page 40
-  Fresh air calibration, refer to page 46
-  Delete peak values, refer to page 19
-  Display pump information, refer to page 23
-  Activate or deactivate pump, refer to page 23


- Press the \oplus key to cancel the active function and to switch to measuring mode.
- If no key is pressed for 60 seconds, the device returns automatically to measuring mode.

Quick menu "Delete peak values"

After the function has been selected, the current peak values are displayed; the peak values special symbol appears in the display at the same time.

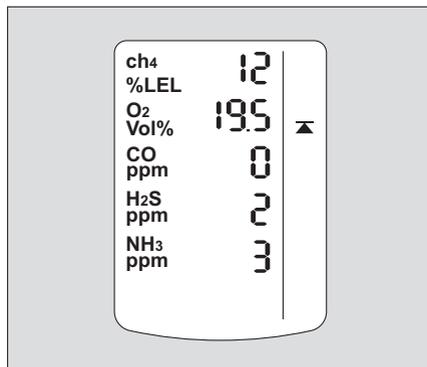


- The peak values can be deleted by pressing the  key for 5 sec. The adjacent display appears.
- Press the  key to end the function.

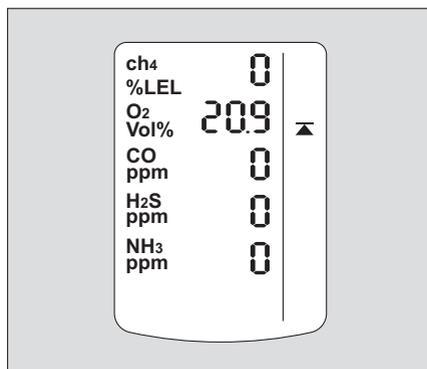

Calling the Calibration Menu

- The calibration menu can only be accessed by entering a password.
Password on delivery: » **001** «
- The default password on delivery can be changed using the PC software Dräger CC Vision.
- In measuring mode, press the **+** key for at least 4 seconds.
- The function for entering the password is selected.
- The » **🔒** « special symbol (for the "enter password" function) is displayed.
- The display shows » **000** «, with the first digit flashing.
- Use the **+** key to set the flashing digit.
- Press the **OK** key, the second digit starts flashing.
- Use the **+** key to set the flashing digit.
- Press the **OK** key, the third digit starts flashing.
- Use the **+** key to set the flashing digit.
- Press the **OK** key to confirm the password once it has been set completely.
- The calibration menu functions can now be selected by pressing the **+** key.
- Press the **OK** key to call the selected function.

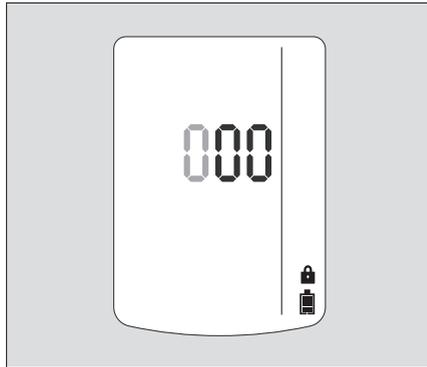

Calibration menu functions

- ✱** Fresh air calibration, refer to page 46
- ↺** 1-button calibration, refer to page 47
- 🔑** Single gas calibration, refer to page 50

- Press the **+** key to cancel the active function.
- If no key is pressed for 10 minutes, the device automatically returns to measuring mode.

Identifying Alarms

An alarm is displayed visually, audibly and through vibration in a specific pattern.

NOTICE
At low temperatures the legibility of the display can be improved by switching on the backlight.

Concentration pre-alarm A1

The alarm is indicated by an intermittent alarm message:



Display » **A1** « and measured value alternating: not for O₂!

- The pre-alarm A1 is not self-latching and stops when the concentration has dropped below the alarm setpoint A1.
- In the case of A1 a single tone is audible and the alarm LED flashes.

Acknowledging the pre-alarm:

- Press the key. Only the audible alarm and the vibration alarm are switched off.

Concentration main alarm A2

The alarm is indicated by an intermittent alarm message:



Display » **A2** « and measured value alternating:

In the case of A2 a double tone is audible and the alarm LED flashes twice.

For O₂: » **A1** « and measured value alternating = oxygen deficiency
 » **A2** « and measured value alternating = oxygen surplus

DANGER
Leave the area immediately. Danger to life! A main alarm is self-latching and cannot be acknowledged or cancelled.

After leaving the area, if the concentration is less than the alarm setpoint A2:

- Press the key. The alarm messages are switched off.

If the measuring range is exceeded significantly on the CatEx channel (very high concentration of flammable materials), a blocking alarm is triggered. This CatEx blocking alarm can be acknowledged manually by switching the device off and back on again in fresh air.

In configuration setting CH₄ with measuring range 100 vol. %, no blocking alarm is triggered as the heat conductance measurement principle is used.

CAUTION
The measuring range 0 to 100 vol. % CH ₄ is not suitable for monitoring explosive mixtures in the measuring range from 0 to 100 %LEL.

STEL / TWA exposure alarm

The alarm is indicated by an intermittent alarm message:



Display » **A2** « and »  « (TWA) or »  « (STEL) and measured value alternating:

⚠ CAUTION

Health hazard! Leave the area immediately. After this alarm, the deployment of personnel is subject to the relevant national regulations.

- STEL and TWA alarms cannot be acknowledged or canceled.
- Switch off the device. The values for the exposure evaluation are deleted after the device is switched on again.

NOTICE

The STEL alarm can be triggered with a maximum delay of one minute.

Battery pre-alarm

The alarm is indicated by an intermittent alarm message:



Flashing special symbol »  « on the right side of the display:

Acknowledging the pre-alarm:

- Press the  key. Only the audible alarm and the vibration alarm are switched off.
- The battery still lasts approx. 20 minutes after the first battery pre-alarm.

Battery main alarm

The alarm is indicated by an intermittent alarm message:



Flashing special symbol »  « on the right side of the display:

The battery main alarm cannot be acknowledged or canceled:

- The device is automatically switched off again after 10 seconds.
- Before the device is switched off, the visual, audible and vibration alarms are activated for a short time.

Device alarm

The alarm is indicated by an intermittent alarm message:



Special symbol »  « on the right side of the display:

- The device or one or several sensor channels are not ready for operation.
- For remedies, refer to page 30 to page 37.
- If necessary, commission the Dräger Service Center to eliminate the error.

Operation with pump

Observe the following when performing measurements using the pump

- Perform visual inspection of the probe, if necessary.
- Wait for the flushing time to end.
Flush the Dräger sampling hose or Dräger probes prior to each measurement with the air sample to be measured.

The flushing phase is necessary to minimize or eliminate any effects associated with the use of a sampling hose or a probe, e.g. memory effects, dead volume. The duration of the flushing phase depends on factors such as type and concentration of the gas or vapour to be measured, material, length, diameter and age of the sampling hose or probe. As a rule of thumb, a typical flushing time of 3 seconds per metre can be assumed for a sampling hose (factory-new, dry, clean). This flushing time applies in addition to the sensor response time (see instructions for use of the gas detector used).

Example:

The flushing time for a 10 m hose is approx. 30 seconds. The sensor response time is approx. 60 seconds in addition. The overall time before reading the gas detector therefore is approx. 90 seconds.

The flow alarm is delayed by 10 to 30 seconds, depending on the hose length.

Performing a measurement with Dräger Pump X-am 1/2/5000

Required accessories (siehe "Accessories" auf Seite 66):

- Dräger Pump X-am 1/2/5000
- Sampling hose and probes

Commissioning and performing the measurement:

- See instructions for use of Dräger Pump X-am 1/2/5000.

Performing a measurement with the Dräger X-am Pump

Required accessories (siehe "Accessories" auf Seite 66):

- Dräger X-am Pump
- Sampling hose and probes

Pump symbols:



Pump battery 100 % charged



Warning for pump
(Gas detector can no longer detect pump.)



Remaining charge of pump
battery: 2/3



Leak test:
Block suction inlet



Remaining charge of pump
battery: 1/3



Leak test:
Release suction inlet



Pump battery discharged

Commissioning and performing the measurement:

- See instructions for use of the Dräger X-am Pump.

Viewing pump information:

- Open the quick menu (siehe "Calling the Quick Menu" auf Seite 18).
- Select  and confirm with the  button.

The following pump information will be displayed:

- serial number
- pump runtime (current operation)
- pump battery charge
- Press the  button to return to measuring mode.

Activating or deactivating the pump:

- Open the quick menu (siehe "Calling the Quick Menu" auf Seite 18).
- Select  or  and activate or deactivate the pump by pressing the  button.
- Press the  button to return to measuring mode.

WARNING

No measurement!

If the pump is connected but deactivated, the gas detector is not ready to measure.
The red LEDs on the gas detector flash.

 **WARNING**

Impairment of accuracy!

After measuring high concentrations of nonane (>20 %LEL), the accuracy for measuring nonane is impaired.

The pump is not suitable for long-term measurement of high concentrations of nonane.

Performing a measurement with a manual pump adapter and rubber ball pump

Required accessories (siehe "Accessories" auf Seite 66):


- Manual pump adapter
- Rubber ball pump
- Sampling hose
- Probes

Commissioning and performing the measurement:

- See instructions for use of the accessories used.

Configuring the Device

To individually configure a device with standard configuration, the device must be connected with a PC.

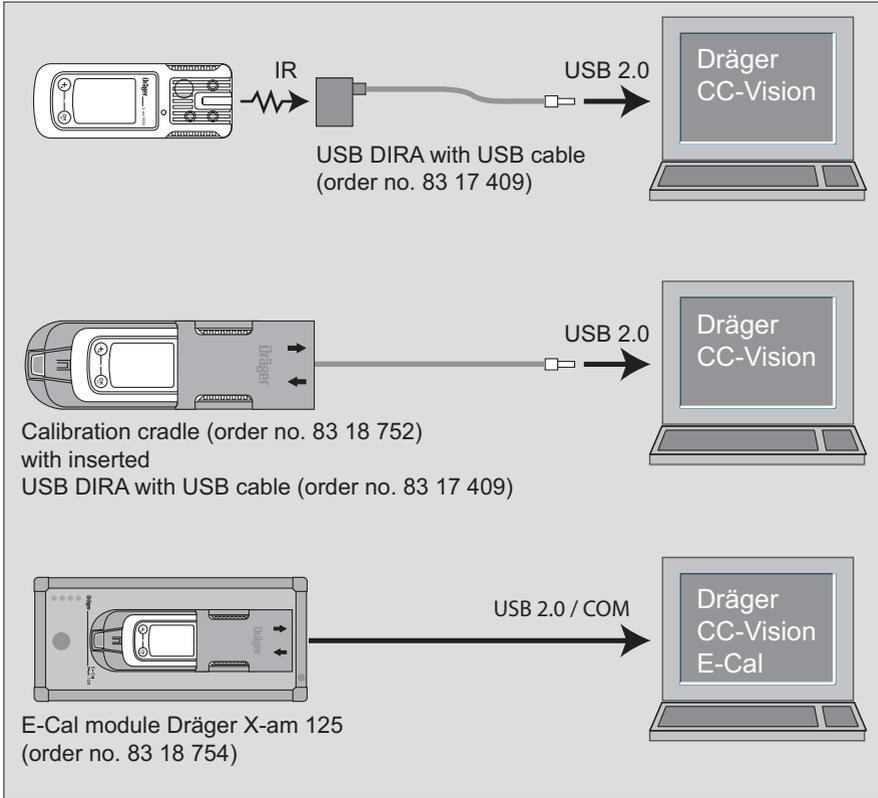

The installed PC software Dräger CC Vision is used for configuration.

- Observe the documentation and online help of the software.
- A version of Dräger CC-Vision which can be used for Dräger X-am 5000 can be downloaded from the following web address: www.draeger.com/software.

Device settings**NOTICE**

Only trained personnel are permitted to make changes to the device configuration.

The following changes can be made to the device parameters for a device:

Designation	Field
Password	Numeric field (3-figure)
Operating signal LED ¹⁾	Yes/No
Operating signal horn ¹⁾	Yes/No
Switch-off mode	“Switch off permitted” or “Switch off prohibited” or “Switch off prohibited at A2”
Shift length (TWA) ²⁾ (in minutes)	60 - 14400 (setting for exposure alarm)
Short-term exposure limit (STEL) ^{3) 4)} (in minutes)	0 - 15 (setting for exposure alarm)
User ID(12 characters)	Alphanumeric field
Switch database on or off	On/Off
Overwrite database	Yes/No
Database mode	Peak/Average
Database interval	1 s / 10 s / 30 s / 1 min / 2 min / 5 min / 10 min / 30 min
Date	(date on the PC)
Time	(time on the PC)
Warning after expiry of calibration interval	Yes/No
Error after expiry of calibration interval	Yes/No
Delay until error after expiry of calibration interval (days)	0 - 10
Automatic detection of Bump Test Station	Yes/No
Activate sensitivity calibration following negative bump test	Yes/No (relates only to a device connected to the Dräger Bump Test Station)
Bump test mode	“extended bump test” or “quick bump test” or “bump test deactivated”
Warning after expiry of bump test interval	Yes/No
Error after expiry of bump test interval (if warning activated)	Yes/No
Capture range	Yes / No
Remote configuration	Yes / No
Bump test interval (days)	1 - 732

Delay until error after expiry of cal. interval (days)	0 - 10
Activate user service life	Yes/No
User service life (days) (if activated)	0 - 999
Running in	Yes/No
LEL category	"---" or "PTB" or "IEC" or "NIOSH" (if this is changed, the LEL factor will be altered to match)

- 1) At least one of the two operating signals must be switched on.
- 2) Corresponds to the averaging time and is used to calculate the exposure value TWA.
- 3) Only evaluated if the sensor is provided for the purpose.
- 4) Corresponds to the averaging time and is used to calculate the exposure value STEL.

Sensor settings

The following changes can be made to the sensor parameters for the sensors:

Designation	Field
Alarm threshold A1 (in measurement unit)	0 - A2
Alarm threshold A2 (in measurement unit)	A1 – Measuring range limit value
Type of evaluation ¹⁾	Inactive, TWA, STEL, TWA+STEL
Alarm threshold STEL (in measurement unit) ¹⁾	0 – Measuring range limit value
Alarm threshold TWA (in measurement unit) ¹⁾	0 – Measuring range limit value
Calibration interval (days)	0 - 180 (sensor-dependent)
Unit (sensor-dependent)	Vol%, %UEG, %LEL, %LIE, ppm, mbar, ppb, mg/m ³
Gas name: "Ex" (CatEx sensor only)	Yes/No
Automatic fresh air calibration in the charging cradle (CatEx sensor only)	Yes / No
ToxicTwins (HCN)	Yes/No

- 1) Only evaluated if the sensor is provided for the purpose.


Testing the parameters

In order to ensure that the values have been correctly transferred to the gas measuring device:

- Press the touch button **Data from X-am 1/2/5x00**
- Check parameters.

Read Database and Display Graphically

To read the database of the device and display it graphically, the device must be connected with a PC.

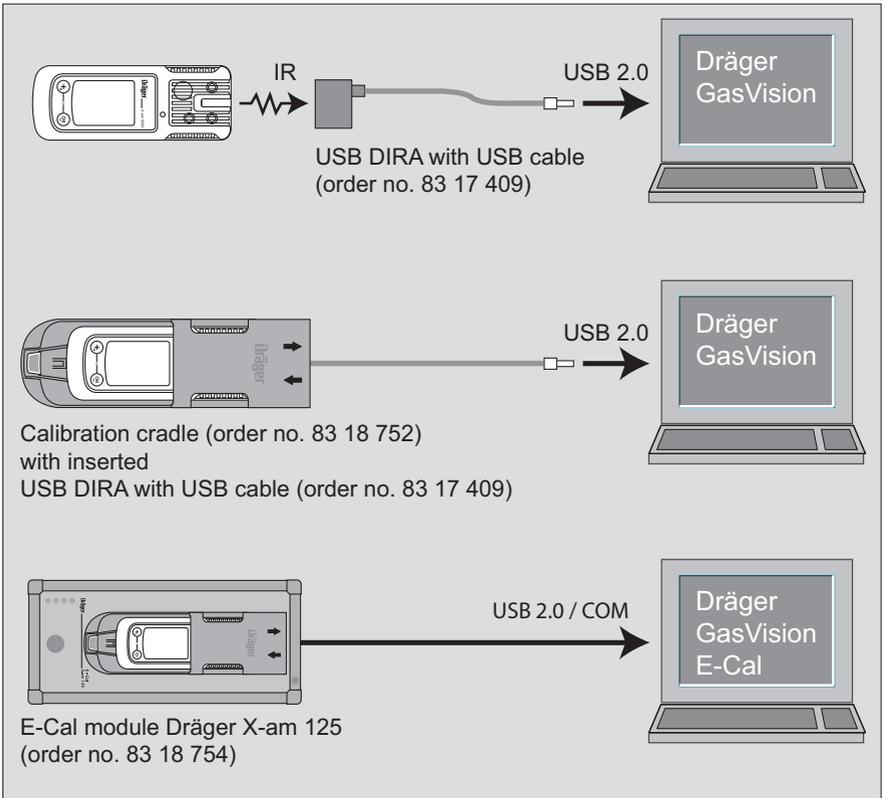

The installed PC software Dräger GasVision is used for reading and displaying the database.

- Observe the documentation and online help of the software.

Faults, Cause and Remedy

Fault	Cause	Remedy
Not possible to switch on the device	Discharge the power pack	Charge the power pack, page 56.
	Discharge the alkaline batteries	Insert new alkaline batteries, page 55.
Not possible to switch off the device	The device is not set to measuring mode	Select measuring mode.
	The device is configured to "Disable prohibited"	Configure the device to "Disable allowed" with Dräger CC Vision.
Display » -- «	Measuring range calibrated incorrectly	Recalibrate the measuring range, page 45.
	Electronics or sensors defective	Must be repaired by DrägerService.

To display the numerical codes of the warning and fault messages in the info mode, page 17.

Warning messages

Special symbol » ⓘ « and displayed numerical code:	Cause	Remedy
152	Customer's service life counter about to elapse	Reset the service life counter using Dräger CC Vision.
153	Database 90 % full	Read the database soon and clear memory afterwards.
154	Database full	Read the database and clear memory.
155	Interval for the function test with gas (bump test) elapsed	Carry out the function test, page 40.
156	Battery pre-alarm of X-am Pump	Recharge the battery soon. The battery will last for at least 20 minutes after the first battery pre-alarm.
159	Calibration not possible. The menu function cannot be carried out because of a message which is preventing the function (e.g., sensors in warm-up phase).	Determine the message code via the info menu and switch it off, if necessary.

Special symbol » ⓘ « and displayed numerical code:	Cause	Remedy
251	DrägerSensor CatEx 125 PR in warm-up phase	Wait until warm-up time is complete.
252	DrägerSensor CatEx 125 PR in warm-up phase	Wait until warm-up time is complete.
253	Ex concentration has drifted into the negative range	Carry out fresh air calibration, page 46.
254	The temperature is too high	Operate the device within the allowed temperature range.
255	The temperature is too low	Operate the device within the allowed temperature range.
256	The calibration interval for DrägerSensor CatEx 125 PR has elapsed	Carry out span calibration for DrägerSensor CatEx 125 PR, page 50.
257	Alarm setpoint A2 setting is greater than 60 %LEL	Set alarm setpoint to less than 60 % LEL.
271	The calibration interval for thermal conduction for DrägerSensor CatEx 125 PR has elapsed	Carry out span calibration for DrägerSensor CatEx 125 PR, page 50.
272	Sensor is switched off due to excess gas	Restart the device

351	DrägerSensor XXS EC1 in the warm-up phase	Wait until warm-up time is complete.
352	DrägerSensor XXS EC1 in the warm-up phase	Wait until warm-up time is complete.
353	EC1 concentration has drifted into the negative range	Carry out fresh air calibration, page 46.
354	The temperature is too high	Operate the device within the allowed temperature range.
355	The temperature is too low	Operate the device within the allowed temperature range.
356	The calibration interval for DrägerSensor XXS EC1 has elapsed	Carry out span calibration for DrägerSensor XXS EC1, page 50.
357	Alarm setpoint A2 setting is greater than 60 %LEL	Set alarm setpoint to less than 60 %LEL.

451	DrägerSensor XXS EC2 in the warm-up phase	Wait until warm-up time is complete.
452	DrägerSensor XXS EC2 in the warm-up phase	Wait until warm-up time is complete.
453	EC2 concentration has drifted into the negative range	Carry out fresh air calibration, page 46.

Special symbol » ⓘ « and displayed numerical code:	Cause	Remedy
454	The temperature is too high	Operate the device within the allowed temperature range.
455	The temperature is too low	Operate the device within the allowed temperature range.
456	The calibration interval for DrägerSensor XXS EC2 has elapsed	Carry out span calibration for DrägerSensor XXS EC 3, page 50.
457	Alarm setpoint A2 setting is greater than 60 %LEL	Set alarm setpoint to less than 60 %LEL.

551	DrägerSensor XXS EC3 in the warm-up phase	Wait until warm-up time is complete.
552	DrägerSensor XXS EC3 in the warm-up phase	Wait until warm-up time is complete.
553	EC3 concentration has drifted into the negative range	Carry out fresh air calibration, page 46.
554	The temperature is too high	Operate the device within the allowed temperature range.
555	The temperature is too low	Operate the device within the allowed temperature range.
556	The calibration interval for DrägerSensor XXS EC3 has elapsed	Carry out span calibration for DrägerSensor XXS EC 3, page 50.
557	Alarm setpoint A2 setting is greater than 60 %LEL	Set alarm setpoint to less than 60 %LEL.
575	Calibration interval for the compensation channel has elapsed	Adjust the sensitivity of the compensation channel.
576	Calibration required because of overgassing.	Adjust the sensitivity of the compensation channel.

651	DrägerSensor XXS EC 4 in the warm-up phase	Wait until warm-up time is complete.
652	DrägerSensor XXS EC 4 in the warm-up phase	Wait until warm-up time is complete.
653	EC 4 concentration has drifted into the negative range	Carry out fresh air calibration, page 46.
654	The temperature is too high	Operate the device within the allowed temperature range.
655	The temperature is too low	Operate the device within the allowed temperature range.

Special symbol » ⓘ « and displayed numerical code:	Cause	Remedy
656	The calibration interval for DrägerSensor XXS EC 4 has elapsed	Carry out span calibration for DrägerSensor XXS EC 4, page 50.
657	Alarm setpoint A2 setting is greater than 60 %LEL	Set alarm setpoint to less than 60 %LEL.

Fault messages

Special symbol » ⚠ « and displayed numerical code:	Cause	Remedy
102	The customer's service life counter has elapsed	Reset the service life counter using Dräger CC Vision.
103	The device is defective	The device must be repaired by DrägerService.
104	Check sum error program code	The device must be repaired by DrägerService.
105	The bump test interval has elapsed	Carry out bump test, page 43.
106	The calibration interval has elapsed (at least 1 calibration interval has elapsed)	Carry out span calibration, page 47 or page 50.
107	Bump test error (at least 1 channel has a bump test error)	Carry out bump test, page 43 or carry out span calibration, page 47 or page 50.
108	The device is defective	The device must be repaired by DrägerService.
109	The menu function cannot be carried out because of an error.	Determine the error code via the info menu and switch it off, if necessary.
111	Failed alarm element test: alarm light.	Repeat alarm element test with Dräger X-dock.
112	Failed alarm element test: alarm horn.	Repeat alarm element test with X-dock.
113	Failed alarm element test: Vibration motor.	Repeat alarm element test with X-dock.
114	Defective parameter check	Correct parameters and repeat test using X-dock
115	Device is disabled by X-dock.	Activate device with X-dock.
116	Failed software update.	The device must be repaired by DrägerService.

Special symbol » ☒ « and displayed numerical code:	Cause	Remedy
117	User parameters not feasible	Check configuration of user parameters and adjust
118	Flow alarm of X-am Pump	Check the gas circuit for obstructions and replace filters if necessary.
121	Overvoltage on X-am Pump	Contact DrägerService.
122	Battery main alarm of X-am Pump	Charge pump.
201	The zero point calibration of DrägerSensor CatEx 125 PR is not valid	Carry out fresh air calibration, page 46.
202	The span calibration of DrägerSensor CatEx 125 PR is not valid	Carry out span calibration, page 47 or page 50.
203	The measurement value of DrägerSensor CatEx 125 PR is in the negative range	Carry out fresh air calibration, page 46.
204	DrägerSensor CatEx 125 PR is not inserted or defective	Check DrägerSensor CatEx 125 PR, page 59.
205	Error during the function test with gas (bump test) of DrägerSensor CatEx 125 PR	Repeat the function test. Calibrate or replace DrägerSensor CatEx 125 PR, if necessary page 59.
207	Failed rise time test.	Repeat rise time test with X-dock.
208	User parameters not feasible	Check configuration of user parameters and adjust
218	Blocking alarm not plausible.	Adjust the sensor.
221	DrägerSensor CatEx 125 PR cannot be operated due to oxygen deficiency	Use in the sensor in an environment containing at least 12 vol. % O ₂ .
222	No valid zero point calibration of DrägerSensor CatEx 125 PR for thermal conduction	Carry out fresh air calibration, page 46.
223	No valid span calibration of DrägerSensor CatEx 125 PR for thermal conduction	Carry out span calibration for thermal conduction, page 47 or page 50.
224	Device incorrectly configured by Dräger CC-Vision.	Change sensor for applicable channel with Dräger CC-Vision.

Special symbol » ☒ « and displayed numerical code:	Cause	Remedy
301	The zero point calibration of DrägerSensor XXS EC1 is not valid	Carry out fresh air calibration, page 46.
302	The span calibration of DrägerSensor XXS EC1 is not valid	Carry out span calibration. Carry out page 50 or fresh air calibration, page 46.
303	The measured value of DrägerSensor XXS EC 1 is in the negative range	Carry out fresh air calibration, page 46.
304	DrägerSensor XXS EC1 is not inserted or defective	Check DrägerSensor XXS EC1, page 59.
305	Error during the function test with gas (bump test) of DrägerSensor XXS EC1	Repeat function test. Calibrate or replace DrägerSensor XXS EC1, if necessary page 59.
307	Failed rise time test.	Repeat rise time test with X-dock.
308	User parameters not feasible	Check configuration of user parameters and adjust
324	Device incorrectly configured by Dräger CC-Vision.	Change sensor for applicable channel with Dräger CC-Vision.
326	Error during warm-up acceleration Dräger Sensor XXS EC1	Disconnect and reconnect power pack or replace the sensor. Sensor must not be loaded with gas within the first 5 minutes.

401	The zero point calibration of DrägerSensor XXS EC2 is not valid	Carry out fresh air calibration, page 46.
402	The span calibration of DrägerSensor XXS EC2 is not valid	Carry out span calibration, page 50.
403	The measured value of DrägerSensor XXS EC 2 is in the negative range	Carry out fresh air calibration, page 46.
404	DrägerSensor XXS EC2 is not inserted or defective	Check DrägerSensor XXS EC2, page 59.
405	Error during the function test with gas (bump test) of DrägerSensor XXS EC2	Repeat function test. Calibrate or replace DrägerSensor XXS EC2, if necessary page 59.
406	Failed filter test.	Repeat filter test with X-dock.
407	Failed rise time test.	Repeat rise time test with X-dock.

Special symbol » ☒ « and displayed numerical code:	Cause	Remedy
408	User parameters not feasible	Check configuration of user parameters and adjust
424	Device incorrectly configured by Dräger CC-Vision.	Change sensor for applicable channel with Dräger CC-Vision.
426	Error during warm-up acceleration Dräger Sensor XXS EC2	Disconnect and reconnect power pack or replace the sensor. Sensor must not be loaded with gas within the first 5 minutes.
501	The zero point calibration of DrägerSensor XXS EC3 is not valid	Carry out fresh air calibration, page 46.
502	The span calibration of DrägerSensor XXS EC3 is not valid	Carry out span calibration, page 50.
503	The measured value of DrägerSensor XXS EC3 is in the negative range	Carry out fresh air calibration, page 46.
504	DrägerSensor XXS EC3 is not inserted or defective	Check DrägerSensor XXS EC3, page 59.
505	Error during the function test with gas (bump test) of DrägerSensor XXS EC3	Repeat function test. Calibrate or replace DrägerSensor XXS EC3, if necessary page 59.
506	Failed filter test.	Repeat filter test with X-dock.
507	Failed rise time test.	Repeat rise time test with X-dock.
508	User parameters not feasible	Check configuration of user parameters and adjust
524	Device incorrectly configured by Dräger CC-Vision.	Change sensor for applicable channel with Dräger CC-Vision.
525	The span calibration for the compensation channel is not valid	Carry out span calibration for compensation electrode.
526	Error during warm-up acceleration Dräger Sensor XXS EC3	Disconnect and reconnect power pack or replace the sensor. Sensor must not be loaded with gas within the first 5 minutes.

Special symbol » ☒ « and displayed numerical code:	Cause	Remedy
601	The zero point calibration of DrägerSensor XXS EC4 is not valid	Carry out fresh air calibration, page 46.
602	The span calibration of DrägerSensor XXS EC4 is not valid	Carry out span calibration, page 50.
603	The measured value of DrägerSensor XXS EC4 is in the negative range	Carry out fresh air calibration, page 46.
604	DrägerSensor XXS EC4 is not inserted or defective	Check DrägerSensor XXS EC4, page 59.
605	Error during the function test with gas (bump test) of DrägerSensor XXS EC4	Repeat function test. Calibrate or replace DrägerSensor XXS EC 4, if necessary page 59.
606	Failed filter test.	Repeat filter test with X-dock.
607	Failed rise time test.	Repeat rise time test with X-dock.
608	User parameters not feasible	Check configuration of user parameters and adjust
624	Device incorrectly configured by Dräger CC-Vision.	Change sensor for applicable channel with Dräger CC-Vision.
626	Error during warm-up acceleration Dräger Sensor XXS EC4	Disconnect and reconnect power pack or replace the sensor. Sensor must not be loaded with gas within the first 5 minutes.

Maintenance

Maintenance intervals

The device should be inspected and maintained by suitably qualified persons annually. Comparisons:

- EN 60079-29-2 – Gas detectors - Selection, installation, use and maintenance of detectors for flammable gases and oxygen
- EN 45544-4 – Electrical apparatus used for the direct detection and direct concentration measurement of toxic gases and vapours - Part 4: Guide for selection, installation, use and maintenance
- National regulations

Recommended calibration interval for measuring channels Ex, O₂, H₂S, SO₂, NO₂ and CO: 6 months.

Calibration interval of other gases: refer to the Instructions for Use of the respective DrägerSensors.

- Depending on device configuration:
 - Replace the alkaline batteries or charge the battery – refer to page 55 to page 56 – after each use, at the latest after the battery alarm has been triggered or after 2 weeks.
- Calibrating the device – page 45.
 - In regular intervals, according to the sensors used and the operating conditions. For sensor-specific calibration data, refer to the Instructions for Use/data sheets of the sensors used¹⁾.
 - Before you carry out safety-related relevant measurements, the zero point and sensitivity of the devices should be tested in accordance with national regulations.
- Inspection by suitably qualified persons – every year.
 - The inspection intervals must be established in each individual case and shortened if necessary, depending on technical safety considerations, engineering conditions and the technical requirements of the equipment.
 - We recommend that a service agreement be concluded with Dräger and that repairs also be carried out by them.
- Replace the sensors, page 59 – if necessary, when it is not possible to calibrate the sensors anymore.

1) Instructions for Use/data sheets for DrägerSensors can be downloaded on the product page of the X-am 5000 at the following Internet address: www.draeger.com. See also the enclosed Instructions for Use and data sheets for the sensors used.

ToxicTwins

When the ToxicTwins feature is activated, the measuring channels of the XXS CO sensor and the XXS HCN sensor are offset against each other in such a manner that the device issues an alarm before the respective A1 alarm threshold is reached if both gases are detected at the same time.

Prerequisites:

- The XXS CO and XXS HCN sensors are installed.
- The ToxicTwins feature is activated (using the Dräger CC-Vision PC software).

If the ToxicTwins feature is activated, HCN+ appears in the measured value display.

CO H₂ compensation

Carbon monoxide (CO) and hydrogen (H₂) can occur simultaneously in workplaces in the steel industry, refineries, sewage works, etc. Hydrogen affects the CO signal in ordinary commercially available sensors, which leads to false alarms. The XXS CO H₂-CP sensor uses two sensing electrodes. One of these electrodes measures CO and H₂, the other one measures only H₂. The difference between the two signals is calculated, so that only the CO value will be displayed. For example, a hydrogen concentration of 1000 ppm (2.5 %LEL) will only result in a maximum of 15 ppm CO being displayed, but the CO alarm will not be triggered.

This feature is automatically available and activated if the XXS CO H₂-CP sensor is installed. Deactivation is not possible.

Prerequisites:


- XXS CO H₂-CP sensor is installed.

If this feature is used, CO+ appears in the measured value display.

Carry out manual bump test

Manual implementation without the documentation of results in the device memory

- Prepare a test gas cylinder, the volume flow must be 0.5 L/min and the gas concentration must be higher than the alarm setpoint concentration to be tested.
Example test gas cylinder 68 11 130 = mixed gas with 50 ppm CO, 15 ppm H₂S, 2.5 vol. % CH₄, 18 vol. % O₂
- Connect the test gas cylinder with the calibration cradle (83 18 752).
- Vent the test gas into a fume cupboard or into the open air (with a hose connected to the second connector of the calibration cradle).

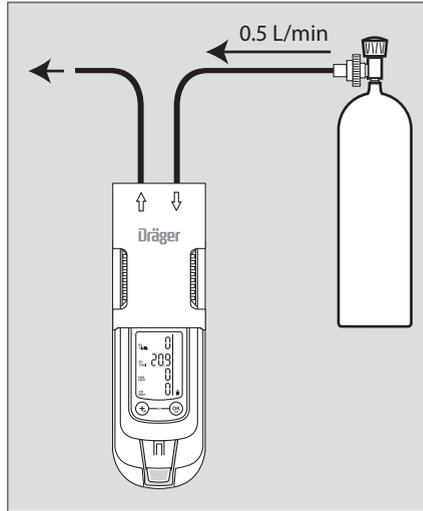

00023999_01_en.eps

⚠ CAUTION

Health hazard! Do not inhale the test gas. Risk to health! Observe the hazard warnings of the relevant Safety Data Sheets.

⚠ WARNING

CSA requirement: carry out a bump test before use. It should be carried out in the measuring range 25-50 % of the full scale value, whereby the displayed measured value may deviate from the actual measured value by 0-20 %. Accuracy may be corrected via calibration.

- Switch on the device and insert it into the calibration cradle – press downwards until it engages.
- Open the test gas cylinder valve to let test gas flow over the sensors.
- Recommendation: Wait until the device displays the test gas concentration with sufficient tolerance –
Ex: $\pm 20\%$ of the test gas concentration ¹⁾
O₂: ± 0.6 vol. % ¹⁾
TOX: $\pm 20\%$ of the test gas concentration ¹⁾.
Wait at least until the alarm setpoint A1 or A2 is exceeded.
- If the alarm setpoints are exceeded, the device displays the gas concentration in alternation with » **A1** « or » **A2** « depending on the test gas concentration.
- Close the test gas cylinder valve and remove the device from the calibration cradle –
– If the concentration has now fallen under the A1 alarm setpoint:
 - Acknowledge the alarm.
 - If the displays are outside of the above-mentioned ranges:

1) Upon application of the Dräger mixed gas (order no. 68 11 130) the displays should be within this range.

- Calibrating the device, refer to page 45.

NOTICE

To check the measured value response times, apply t90 test gas to the X-am via the calibration cradle. Check the results in accordance with the information in the table in the enclosed supplementary documentation (order no. 90 33 890) until 90 % of the end display is reached.

NOTICE

After the bump test, the display shows a printer icon even if there is no printer connected to the bump test station.

Menu implementation with the documentation of results in the device memory

The "Quick bump test" or the "Extended bump test" is selected using the Dräger CC Vision PC software. The "Quick bump test" checks whether the gas concentration has exceeded the Alarm 1 threshold (with oxygen, the check is whether the concentration has fallen below the Alarm 1 threshold). In the case of the "Extended bump test", a check is made as to whether the gas concentration has reached the set bump test concentration within a tolerance window.

Setting on delivery: Extended bump test.


- Prepare a test gas cylinder, the volume flow must be 0.5 L/min and the gas concentration must be higher than the alarm setpoint concentration to be tested. Example test gas cylinder 68 11 130 = mixed gas with 50 ppm CO, 15 ppm H₂S, 2.5 vol. % CH₄, 18 vol. % O₂
- Connect the test gas cylinder with the calibration cradle (83 18 752).
- Vent the test gas into a fume cupboard or into the open air (with a hose connected to the second connector of the calibration cradle).

⚠ CAUTION


Do not inhale the test gas. Risk to health!

Observe the hazard warnings of the relevant Safety Data Sheets.

- Switch on the device and insert it into the calibration cradle – press downwards until it engages.
- Call the quick menu and select the function test with gas (bump test), page 18.

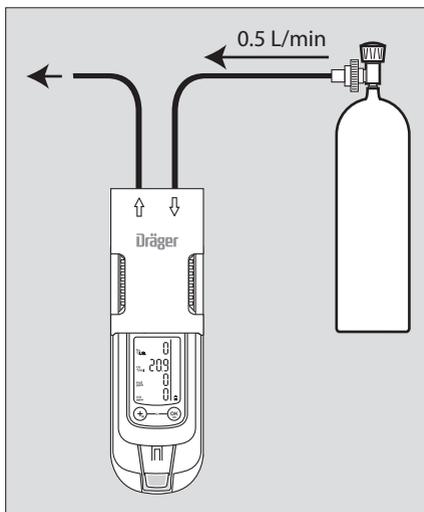


- The current gas concentration values and the special symbol » √∩ « (for bump test) flash.
- Press the **OK** key to start the function test with gas.
- Open the test gas cylinder valve to let test gas flow over the sensor.
- If gas concentration exceeds the alarm thresholds A 1 or A 2 the corresponding alarm will occur. Exit the function test with gas:

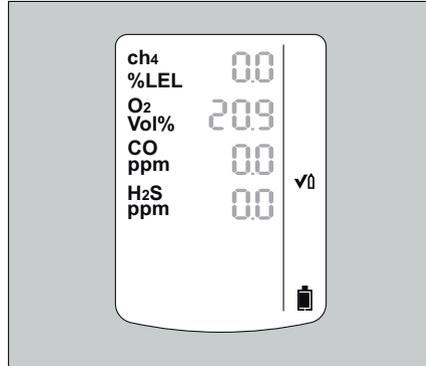

02423999_01_en.eps

After the preset bump test concentration is reached or a gas alarm is triggered (with the "Quick bump test"):


- The display containing the current gas concentration changes with the display » **OK** «.
- The bump test that was carried out is documented with the result and date in the device memory.
- Close the test gas cylinder valve and remove the device from the calibration cradle.
- If the concentration values have now fallen under the A1 alarm setpoints, the device returns to the measuring mode.

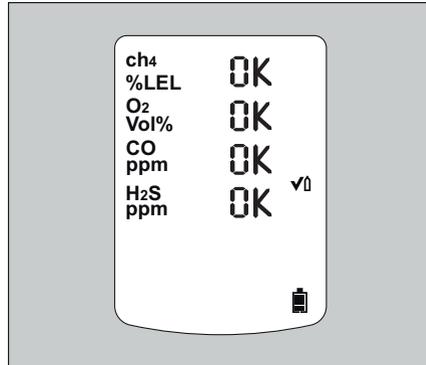

02523999_01_en.eps

- If the set bump test concentration is not reached within the specified time, the alarm mode is activated to indicate failure.
- The fault message » **X** « appears and » - - « is displayed instead of the measured value on the faulty measuring channel.
- In this case, repeat the function test with gas or calibrate the device, page 45.

The function test with gas can also be carried out automatically. The "Bump Test Station" is required for this function, refer to page 43.

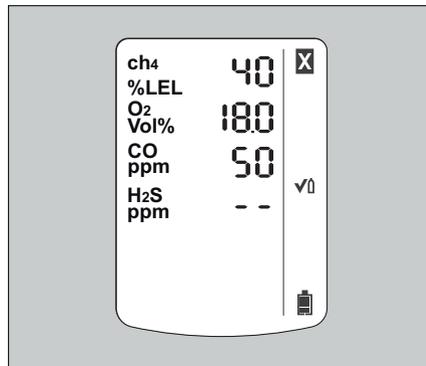


02623999_01_en.eps

Automatic implementation with the Bump Test Station


Prerequisite:

The device must first be configured for the automatic function test with gas (bump test) using the PC software Dräger CC Vision.

- Activating the device for the automatic function test.
 - Adjust the test gas concentration (mixed gas) with the Dräger CC-Vision PC software if it deviates from the following default values – standard on delivery: 50 ppm CO, 15 ppm H₂S, 2.5 vol. % CH₄, 18 vol. % O₂
 - Define which measuring channels should participate in the automatic function test. All measuring channels participate in the function test by default.
- Prepare the Bump Test Station according to the instructions.
 - Switch on the device and insert it into the receptacle of the Bump Test Station until it engages.

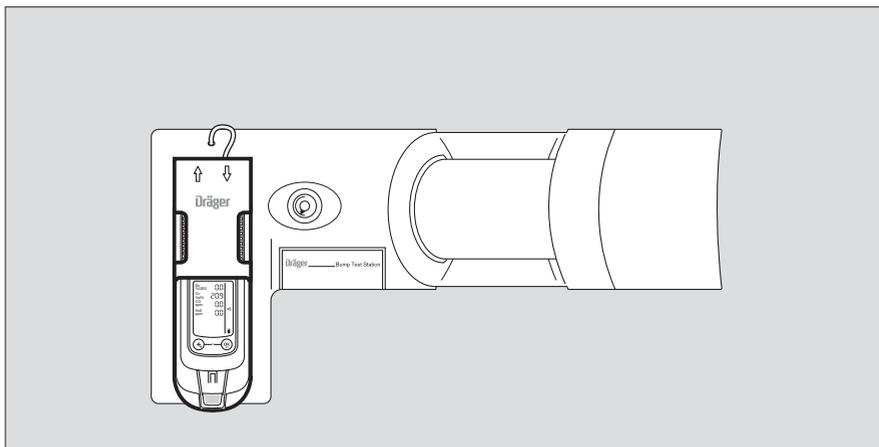


- The function test with gas is started automatically. The special symbol » √ ‹ (for bump test) flashes.
- If a gas alarm (Quick bump test) is triggered and the preset bump test concentration (Extended bump test) is reached within the specified time, the display shows the current gas concentration, alternating with » OK ‹.

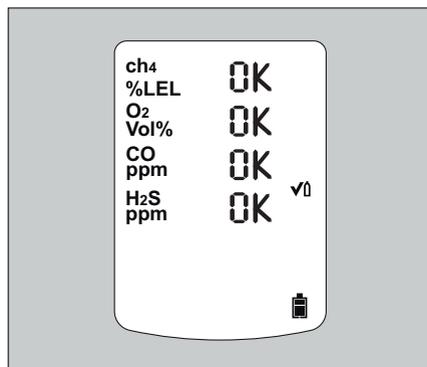

03823999_01.eps

0323999_01_en.eps

- Remove the device from the Bump Test Station.
- If the concentration values have now fallen under the A1 alarm setpoints, the device returns to the measuring mode.
- An error will be triggered if the preset bump test concentration is not reached within the specified time.
- The fault message »  « appears and » - - « is displayed instead of the measured value on the faulty measuring channel.
- In this case, repeat the function test with gas or calibrate the device, page 45.

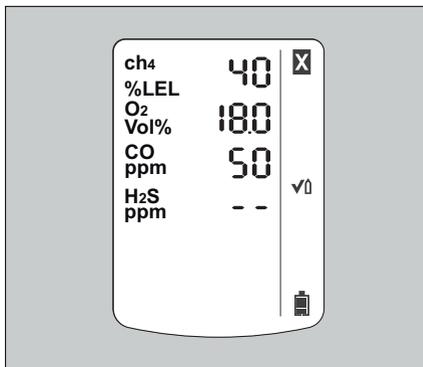

The function test with gas can also be carried out manually, refer to page 40.

The PC program Dräger CC Vision can be used to enable the "Automatic calibration after incorrect bump test" option.

NOTICE

After the bump test, the display shows a printer icon even if there is no printer connected to the bump gas station.

Calibrating the Device

NOTICE

Dräger recommends using the extended bump test for cross calibrations (Dräger X-dock technical manual).

Calibration may not be possible due to device and channel errors.

Allow the sensors to warm up before the calibration!

Warm-up time: see Instructions for Use/data sheets of the installed DrägerSensors (at www.draeger.com).

Calibration interval:

- Observe the relevant specifications in the Instructions for Use/data sheets of the DrägerSensors installed.
- For critical applications, observe the recommendations in EN 60079-29-2¹⁾ or EN 45544-4²⁾ and national regulations. We recommend that you calibrate the channels after 6 months.

⚠ CAUTION

Do not inhale the test gas. Risk to health!

Observe the hazard warnings of the relevant Safety Data Sheets.

- Improve the zero point accuracy – carry out the fresh air calibration, page 46.
- Set the sensitivity of all sensors to the value of the test gas – carry out the 1-button calibration, page 47.
- Set the sensitivity of a sensor to the value of the test gas – calibrate the sensitivity, page 50.

1) EN 60079-29-2 – Gas measuring device - Selection, installation, use and maintenance of apparatus for the measurement of combustible gases or oxygen

2) EN 45544-4 – Electrical devices for the direct detection and direct concentration measurement of toxic gases and vapors – Part 4: Guidelines for selection, installation, use and maintenance.

Carrying out the fresh air calibration

To improve the zero point accuracy, you can carry out a fresh air calibration.


NOTICE

If none of the sensors fitted permits calibration with fresh air (e.g. only O₃, only IR-CO₂), fresh air calibration is not offered as a menu function.

- Calibrate the device to fresh air, free of measured gases or other interfering gases.
- Not all sensors are included in the fresh air calibration¹⁾. Sensors which have not warmed up or which are faulty prevent a calibration.
In the case of sensors which are in the warm-up phase, the message » 159 « is displayed with the special symbol »  « (for warning message).
In the case of a sensor or device error, the message » 109 « is displayed with the special symbol »  « (for a fault message).
The message is cleared after 5 seconds and the function is available again in the menu
- During the fresh air calibration, the zero point of all sensors (with the exception of DrägerSensor XXS O₂) is set to 0.
In the case of DrägerSensor XXS O₂, the display is set to 20.9 vol. %.
- Switch on the device.

Depending on device configuration:


- Call the quick menu and select the Fresh Air Calibration function, page 18.
or
- Call the calibration menu and select the Fresh Air Calibration function, page 20.
- The current gas concentration values flash.
When the measured values have stabilized:
- Press the  key to perform the fresh air calibration.

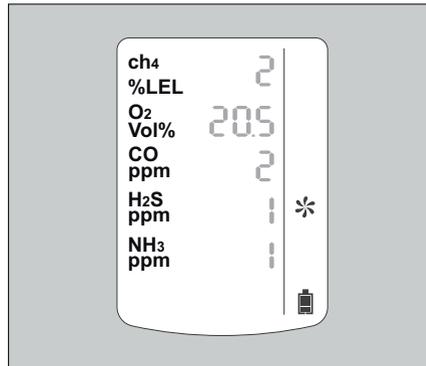

03123999_01_en.eps

1) Fresh air calibration / zero point calibration is not supported by the DrägerSensor XXS O₃. A zero point calibration / adjustment of these sensors can be conducted using the Dräger CC-Vision PC software. To do so, a suitable zero gas that is free of ozone (e.g. N₂) should be used.


- The display containing the current gas concentration changes with the display » **OK** «.
- Press the (OK) key to confirm the calibration or wait for approx. 5 seconds.

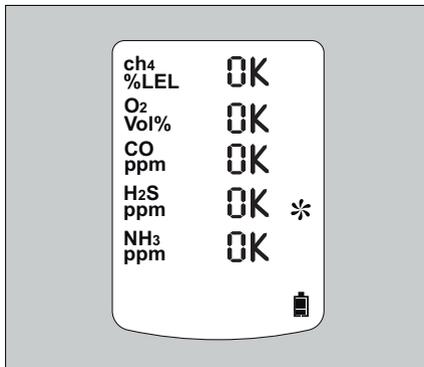

0323999_01_en.eeps

If a fault occurred during the fresh air calibration.

- The fault message »  « appears and » - - « is displayed for the respective sensor instead of the measured value.
- In this case, repeat the fresh air calibration.
- If necessary, replace the sensor, page 59.

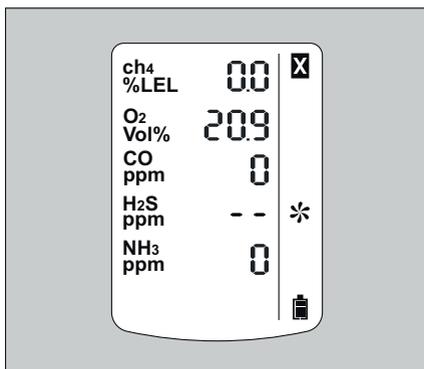

0323999_01_en.eeps

NOTICE

Automatic surrogate calibration

If the corresponding gas combination and the sensor are approved to do so, an automatic surrogate calibration and tests can be performed using the PC software Dräger CC-Vision¹⁾.

A gas for the bump test, for the adjustment and the measured gas can be set in the gas change wizard in Dräger CC-Vision.

Conversions are performed automatically and no longer need to be made manually. The settings are also used by the Dräger X-dock.

1) The PC software Dräger CC Vision can be downloaded from the following web address free of charge: www.draeger.com/software

Automatic fresh air calibration of the CatEx sensor in the charging cradle

This feature is used to perform an automatic fresh air calibration of the CatEx sensor after placing it in the charging cradle. The feature can be adjusted using the Dräger CC-Vision PC software.

NOTICE

If the automatic fresh air calibration feature of the CatEx sensor is activated, the user must ensure that the charging cradle remains in normal atmosphere (21 vol.% O₂) free of contaminants for the entire duration of the process.

Carrying out 1-button calibration


NOTICE

If no sensors are enabled for 1-button calibration by the Dräger CC Vision PC program, the 1-button calibration menu function will not be offered.

- All sensors that are enabled by the Dräger CC Vision PC program take part in the 1-button calibration.
- In the case of the 1-button calibration, the sensitivity of all sensors is set to the value of the test gas.
When using the test gas cylinder 68 11 130 = mixed gas with 50 ppm CO, 15 ppm H₂S, 2.5 vol. % CH₄, 18 vol. % O₂.
- If a mixed gas with another composition is used, the specified concentration values in the device must be changed to the target values of the mixed gas used using the PC software Dräger CC Vision.
- Connect the test gas cylinder with the calibration cradle.
- Vent the test gas into a fume cupboard or into the open air (with a hose connected to the second connector of the calibration cradle).


CAUTION

Health hazard! Do not inhale the test gas. Risk to health!
Observe the hazard warnings of the relevant Safety Data Sheets.

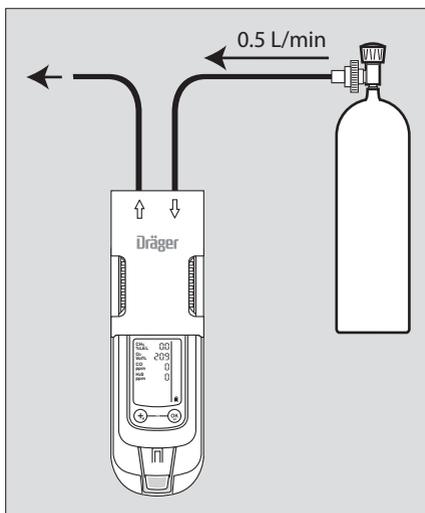

02723999_01_enraps

- Switch on the device and insert it into the calibration cradle until it engages.
- Call the calibration menu, enter the password and select the 1-button calibration function, page 20.
- Press the **OK** key to start the 1-button calibration.

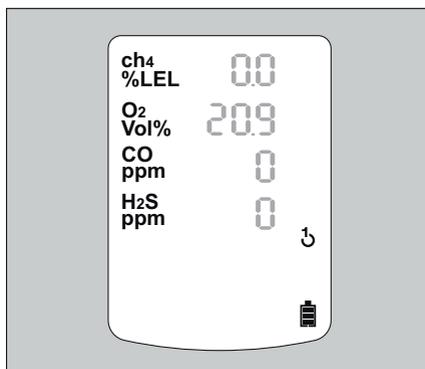

02823999_01_enraps

- Open the test gas cylinder valve to let test gas flow over the sensor.
- The currently displayed measured values start to flash.
- The flashing stops after a static measured value has been reached.
- The calibration is now carried out automatically.
- The displayed measured values change to the values according to the gas supplied.
- The automatic stability monitoring can be overridden by pressing the OK key. A calibration then takes place immediately. If it is detected that no test gas has been applied, the 1-button calibration will be aborted. The channels will then indicate » n/a «. If only one sensor is taking part in the 1-button calibration, a calibration will be performed in each case when the OK key is pressed.


When the calibration is completed and the displayed measured values have stabilized:

- The display containing the current gas concentration changes with the display » **OK** «.
- Press the **OK** key or wait for 5 seconds to quit the calibration.
- The device changes to the measuring mode
- Close the test gas cylinder valve and remove the device from the calibration cradle.



If a fault occurred during the 1-button calibration.

- The fault message » **✖** « appears and » **- -** « is displayed for the respective sensor instead of the measured value.
- In this case, repeat the 1-button calibration or carry out a single gas calibration, refer to page 50.
- If necessary, replace the sensor, page 59.

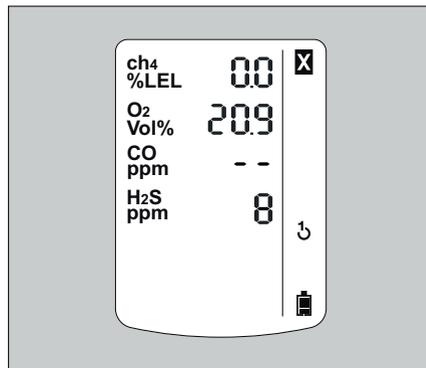

Calibrating the sensitivity for an individual measuring channel

- The span calibration can be carried out specifically for individual sensors.
- In the case of the span calibration, the sensitivity of the selected sensor is set to the value of the test gas used.
- Use a standard test gas.

Allowed test gas concentration:

Ex: 40 to 100 %LEL

O₂: 10 to 25 vol. %


CO: 20 to 999 ppm

H₂S: 5 to 99 ppm

NO₂: 5 to 99 ppm

Test gas concentration of other gases:
refer to the Instructions for Use of the
respective DrägerSensors.

- Connect the test gas cylinder with the calibration cradle.
- Vent the test gas into a fume cupboard or into the open air (with a hose connected to the second connector of the calibration cradle).

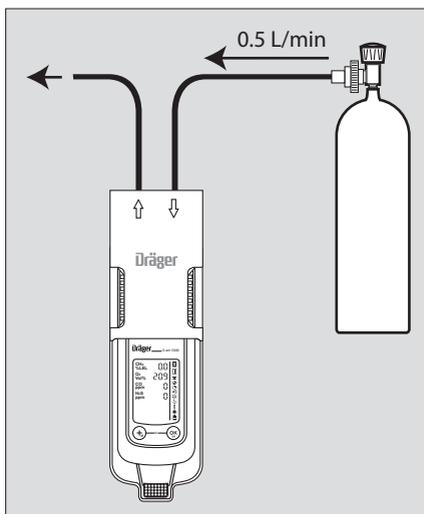


0272399_01_en.eps

⚠ CAUTION

Health hazard! Do not inhale the test gas. Risk to health!
Observe the hazard warnings of the relevant Safety Data Sheets.

- Switch on the device and insert it into the calibration cradle.
- Press and hold the [+] key for 5 seconds to call the calibration menu, enter the password and select the single gas calibration function, page 20.
- Press the **OK** key to start the channel selection.
- The display flashes the gas of the first measuring channel, e.g., » Ex - %LEL «.
- Press the **OK** key to carry out the calibration of this measuring channel, or
- Use the **+** key to select another measuring channel (O₂ - vol. %, H₂S - ppm or CO - ppm).

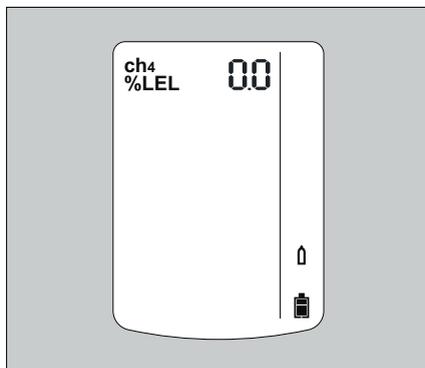


0352399_01_en.eps

Span calibration for CatEx

- If the measuring range end value $\leq 100\%LEL$, the adjustment for the heat tinting is offered.

Display in the case of channel selection:


- Open the test gas cylinder valve to let test gas flow over the sensor.
- Press the **OK** key to start the calibration for the heat tinting or press the **+**-key to select the next sensor.

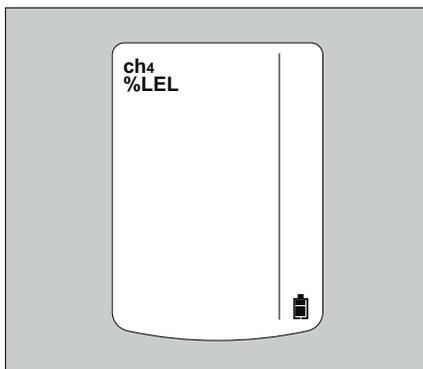

05823999_en.eps

If the displayed measurement value is stable:

- Press the **OK** key to perform the calibration.
- The display containing the current gas concentration changes with the display » **OK** «.
- Press the **OK** key or wait for approx. 5 seconds to end the calibration of this measuring channel.
- The next measuring channel is offered for calibration.
- After the calibration of the last measuring channel, the device changes to measuring mode.

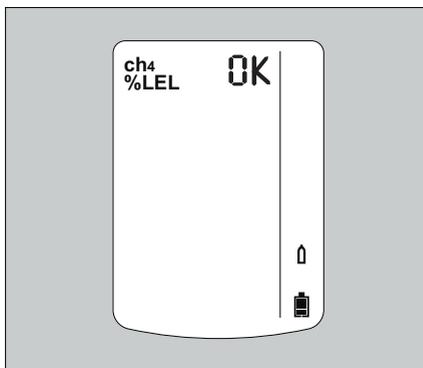


03623999_01_en.eps

- Close the test gas cylinder valve and remove the device from the calibration cradle.


If a fault occurred during the span calibration.

- The fault message »  « appears and » - - « is displayed for the sensor instead of the measured value.
- In this case, repeat the calibration.
- If necessary, replace the sensor, page 59.

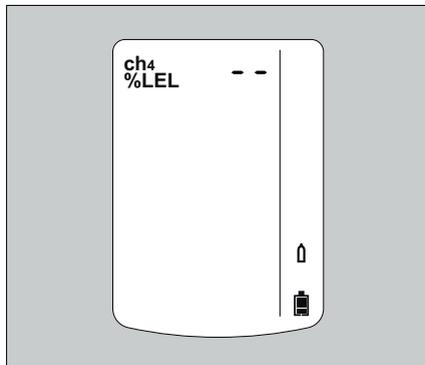

0372399_01_en.eps

- If the gas CH₄ (measurement range up to 100 vol. %) is selected on the CatEx channel, the heat conductivity is calibrated, display with channelselection:

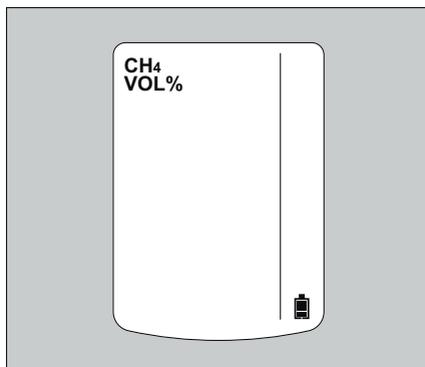

0512399_01_en.eps


- Press the  key to perform the calibration for heat conductivity.

- Press the  key to select the next sensor.

- Press the  key to perform the calibration of the selected measuring channel.

- The test gas concentration is displayed.

- Press the  key to confirm the test gas concentration or use the [+] key to change the test gas concentration and complete the process by pressing the  key.
- The measurement value flashes.

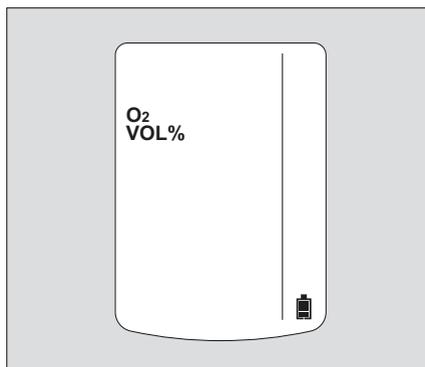

0622399_01_de.eps

- Open the test gas cylinder valve to let test gas flow over the sensor.

- The displayed, flashing measurement value changes to the value according to the supplied test gas.

- Press the  key to select the next sensor.

Note on the use in underground mining:

- When calibrating the Ex channel to methane as the measured gas, the indication on the instrument must be set to a value 5 % (relative) higher than the test gas concentration used.

Automatic fresh air calibration in the charging cradle (CatEx sensor only):

Calibrate the gas detector to fresh air, free of measured gases or other interfering gases. If the function is selected, a fresh air calibration of the CatEx sensor is performed automatically as soon as the gas detector is inserted in the charging cradle. This function can be selected or disabled using the CC-Vision PC software.

No calibration takes place if the warm-up is not yet complete:

- Alarm LED is illuminated red.
- The acoustic signal sounds twice followed by three short tones and the gas detector switches off.

Once the fresh air calibration has been successfully completed:

- Alarm LED is illuminated red.
- The acoustic signal sounds once followed by three short tones and the gas detector switches off.

If a fault has occurred during the fresh air calibration:

- The fault message  appears and  is displayed for the respective sensor instead of the measured value.
- In this case, repeat the fresh air calibration.
If necessary, have the sensor replaced by qualified personnel.

Replacing the batteries / rechargeable batteries

⚠ WARNING

Explosion hazard! To reduce the risk of flammable or explosive atmospheres igniting, it is essential that the warning notices below are observed:

Do not throw used batteries into fire or try to open them by force.

Do not replace or charge batteries in areas at risk of an explosion hazard.

Do not mix new batteries with used batteries, and do not mix batteries from different manufacturers or of different types.

Remove batteries before maintenance work.

Batteries / rechargeable batteries are part of the Ex approval.


Only the following types may be used:

- Alkaline batteries – T3 – (non rechargeable!)
Panasonic LR6 Powerline,
Varta Type 4106¹⁾ (power one) or
Varta Type 4006¹⁾ (industrial)
- Alkaline batteries – T4 – (non rechargeable!)
Duracell Procell MN1500¹⁾, Duracell Plus Power MN1500¹⁾
- NiMH rechargeable batteries – T3 – (rechargeable)
GP 180AAHC¹⁾ (1800) max. 40 °C ambient temperature.

1) Not subject to the Metrological Performance Test BVS10 ATEX E 080X and PFG 10 G 001X.

Switching off the device:

- Press and hold the  key and the  key at the same time.
- 1 Loosen the screw (2.0 mm hexagon socket) on the power pack and remove the power pack.
 - 2 Replace the alkaline batteries with new ones or the rechargeable NiMH batteries with charged ones – **ensure correct polarity**.
 - 3 Completely replace the power pack T4 (with sealed rechargeable batteries, order no. 83 18 704).
- Insert the power pack into the device and tighten the screw, the device switches on automatically.

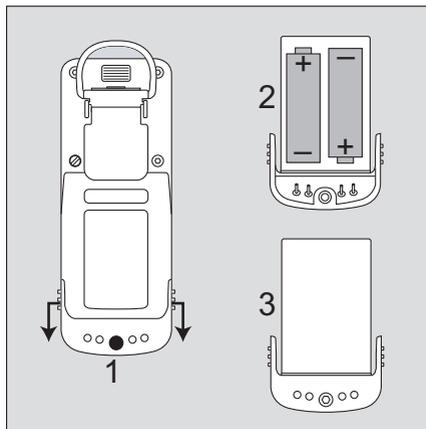

01623998_01 eps

After replacing the power pack T4, it is recommended that a complete charging is carried out.

After the batteries have been replaced:

- The settings and data are stored when the battery is replaced. The sensors warm up again.

Charging the rechargeable batteries

WARNING

Explosion hazard! To reduce the risk of flammable or explosive atmospheres igniting, it is essential that the warning notices below are observed:
Do not charge underground or in explosion-hazard areas! Danger of explosion!
The chargers are not designed in accordance with the regulations for firedamp and explosion protection.
Charge the NiMH power pack T4 (HBT 0000 type) or T4 HC (HBT 0100 type) using the corresponding Dräger charger. Ambient temperature during the charging process: 0 to +40 °C.

Even if the device is not used, we recommend that you store the device in the charger (Charging module X-am 1/2/5000, order no. 83 18 639)!

To maintain the lifetime of the batteries, charging is temperature controlled and only performed in a temperature range of 5 to 35 °C.

When this temperature range is left, the charging process is automatically interrupted and automatically continued after the temperature range has been reached again.

The charging time is typically 4 hours.


A new NiMH power pack reaches its full capacity after three complete charging/discharging cycles. Never store the device for extended periods without being connected to a power source (maximum of 2 months) because the internal buffer battery will drain.

Charging with the multiple charging station

- A maximum of 20 devices can be charged at the same time on the power pack (order no. 83 18 805) of the multiple charging station.
- When attaching the charging modules, disconnect the power pack from the mains supply!

Attaching charging modules

- 1 Turn the slots of the interlock into a horizontal position by using a screwdriver or coin.
- 2 Insert the projecting tongue of the charging module (at the same time, current entry) until it engages.
- 1 Close the interlock with a quarter turn (slot is positioned vertically).

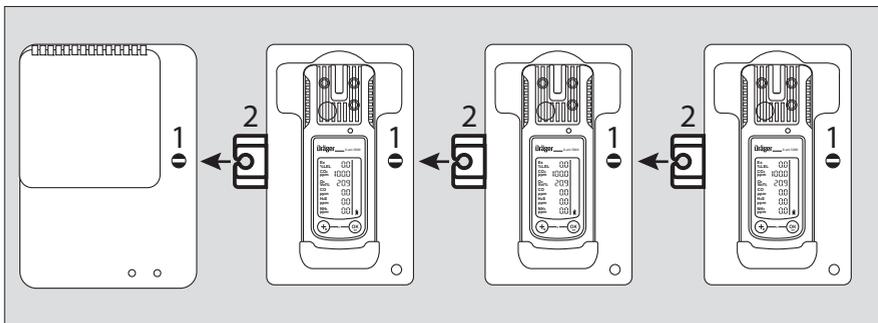

00723999_01_en.eps


- Attach additional charging modules in the same way.
- Always connect or disconnect the charging modules individually and not in groups in order to prevent the charging station from becoming damaged. During transportation, the power pack and the charging modules should also always be handled individually and without inserted devices.

- Position the device on an even and level surface.

- Connecting the power pack to the mains.

- 1 The green "Mains" LED lights.
- Insert the device into the charging module.


- 2 Display LED on the charger:



If a fault occurs:

Remove the device from the charging module and insert it again.

If the fault still occurs, have the charging module repaired.

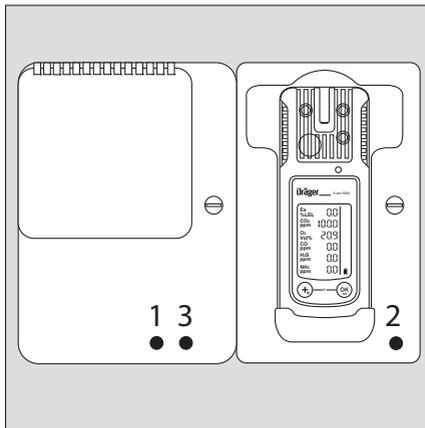

00823999_01_en.eps

It takes approx. 4 hours to fully charge an empty rechargeable battery.


A short circuit of the charging contacts in the charging modules, e.g., by metallic objects that have fallen in, does not result in damage to the charging station. It should, however, be avoided due to possible heating hazards and incorrect displays on the charging module.

In the event of a short circuit or if the power pack is overloaded:

- 3** The red "Overload" LED lights, and an audible alarm sounds.
- After the fault has been corrected, the alarm is switched off automatically and the charging process is restarted.
 - In the event of a power failure, the devices already charged will be protected from discharging.

Charging with charging module and plug-in power pack or vehicle charging adapter

- When using the power pack (order no. 83 16 994), up to 5 devices can be charged at the same time, with power pack (order no. 83 15 635) up to 2 devices.
- The power pack contained in the rechargeable battery and charging set (order no. 83 18 785) is suitable for charging a device.
- When using the vehicle charging adapter (order no. 45 30 057) it is recommended that you supply every charging module separately.

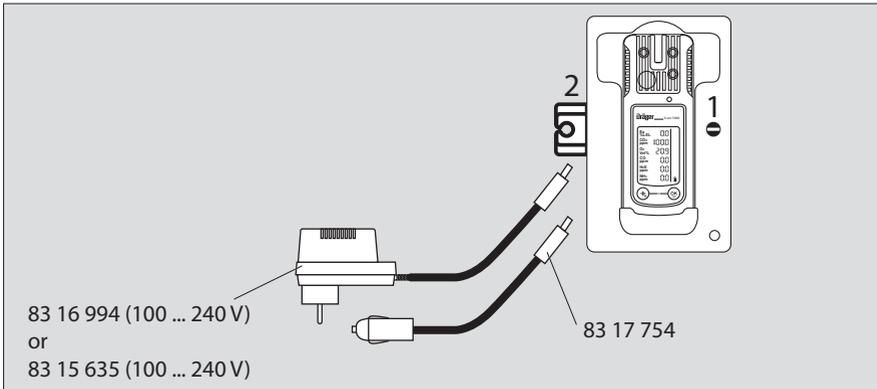

The charging process is carried out analog to charging with the multiple charging station.

Replacing the Sensors

⚠ CAUTION


⚠ Damage to components!

There are components in the instrument that are sensitive to electric charge. Before opening the instrument to replace the sensor, ensure that the person performing the work is earthed to avoid damage to the device. Earthing can be safely ensured, e. g. via an ESD workstation (electrostatic discharge).

NOTICE

To open the instrument, unfasten the casing screws using a screwdriver (Torx T6).

- To replace the sensors of the device, connect the device with a PC.
- Replace the sensors using the PC program Dräger CC Vision.

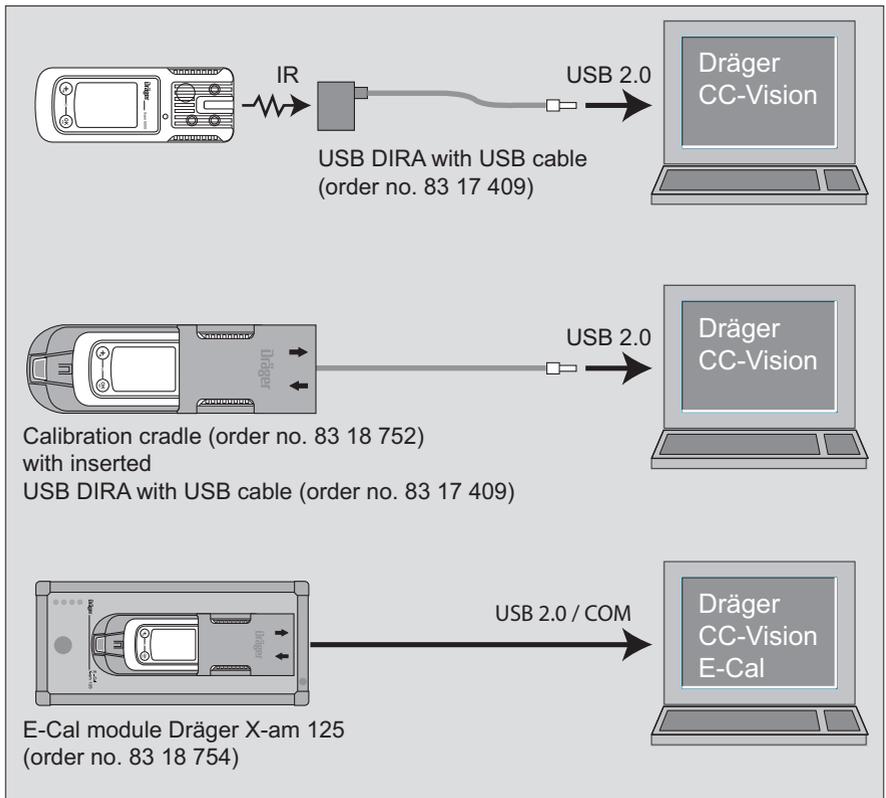

Next:

- Carry out a fresh air calibration, page 46.
- and then:
- Calibrate the sensitivity:
either
carry out 1-button calibration, page 47
or
carry out span calibration, page 50.

Electrochemical sensors

WARNING

Do not throw into fire,
Do not force open. Danger! Acid burn risk!
Sensors of type XXS O₃ and XXS NO₂ LC contain small quantities of nanomaterials.



Like batteries, only dispose of as special waste, in accordance with local waste disposal regulations. Further information can be obtained from the relevant local authority and from appropriate waste disposal companies.

The DrägerSensor CatEx 125 PR should be disposed of as electronic waste.

Sensor warm-up acceleration

There is a function available for accelerating the warm-up procedure for selected EC sensors. The function shortens the time taken until the unit is ready to make measurements, i.e. the time taken to save the display and alarm evaluation of the measurements. The time to activate the calibration is not changed.

- In order to use the sensor warm-up acceleration function in the Dräger X-am 5000, at least one sensor suitable for the purpose must be fitted and registered in the unit using the Dräger CC-Vision PC software.
- After that, activate the function by ticking the "Accelerated warm-up" checkbox ("Device" menu) and updating the device data with Dräger CC-Vision.

NOTICE


A selection menu for activating the process will only be displayed after the device is restarted by plugging in a power pack.

- Restart the device by plugging in a power pack.
 - All the display segments, including the visual, audible and vibration alarms, are activated for a short time.
 - The software version is displayed.
 - The instrument performs a self test.
 - The sensor warm-up acceleration menu is displayed.

The steps in the selection menu are limited by a 25-second time-out, which then changes to the standard setting of unaccelerated warm-up and proceeds with the device start-up procedure.
- It is necessary to select between two times for the sensor warm-up acceleration,
 - the shortened time achievable as a result of the warm-up acceleration,
 - the unshortened time required by the installed sensors to save the measurement display (measurement does not flash any more).
- Select the shortened warm-up time with the **+** button and confirm it with the **OK** button.
 - The function for entering the password is called up.
- Enter the digits with the **+** button and confirm with the **OK** button.



05523999_01.eps

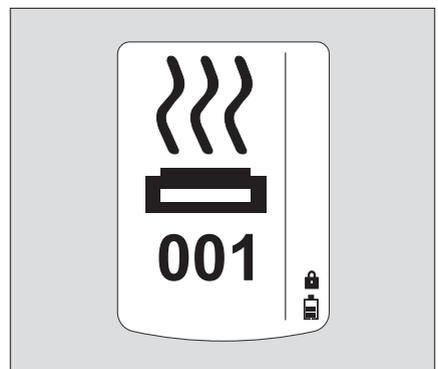

05623999_01.eps

- Start of the warm-up acceleration.
- The remaining time is displayed and decremented.

▲ WARNING

This function requires that the device is in a gas-free environment. A warning screen is displayed and the remaining time during which no gas may be applied is shown. It is essential to ensure that the sensor is in the fresh air during this time (for approx. 5 minutes)! Any gas applied during this period could later result in faulty alarms or suppressed alarms!



05723999_01.eps

If the procedure is unsuccessful, e.g. as a result of a defective sensor, this will be indicated by error code » X07 « on the channel for the affected sensor (X). In the event of a fault, the device will also switch to the unaccelerated mode.

Dräger recommends that the device not be switched off and on again for a period of two hours when the accelerated warm-up is in use.

Cleaning

The device does not need any special care.

- Dirt and deposits can be removed from the device by washing it with cold water. A sponge can be used for wiping if necessary.

▲ CAUTION

Abrasive cleaning implements (brushes etc.), cleaning agents and cleaning solvents can destroy the dust and water filters.

- Carefully dab dry the device using a cloth.

Storage

- Dräger recommends storing the instrument in the charger module (order no. 83 18 639).
- Dräger recommends checking the charge of the power supply at least every three weeks if the instrument is not stored in the charger module.

Disposal



This product must not be disposed of as municipal waste. This is indicated by the adjacent icon.

You can return this product to Dräger free of charge. For information please contact the national sales organisations and Dräger.



Batteries and rechargeable batteries must not be disposed of as municipal waste. This is indicated by the adjacent icon. Collect and dispose of batteries and rechargeable batteries at battery collection centres, in accordance with applicable regulations.

Technical Data

X-am 5000

Ambient conditions:	
during operation and storage	<p>Temperature class T4 (-20 to +50 °C): NiMH power packs type: HBT 0000, HBT 0100 Power pack type: ABT 0100 with alkaline single cell type: Duracell Procell MN 1500¹⁾, Duracell Plus Power MN 1500¹⁾</p> <p>Temperature class T3 (-20 to +40 °C): Power pack type: ABT 0100 with NiMH single cell type: GP 180AAHC¹⁾ with alkaline single cell type: Panasonic LR6 Powerline</p> <p>Temperature class T3 (0 to +40 °C): Power pack type: ABT 0100 with alkaline single cell type: Varta 4006¹⁾, Varta 4106¹⁾</p>
Temperature range over a short period (ATEX & IECEx only) ¹⁾ :	<p>-40 to +50 °C Maximum of 15 minutes with NiMH power pack T4 (HBT 0000) or T4 HC (HBT 0100) Prerequisite: storage of the instrument at room temperature (+20 °C) for at least 60 minutes in advance.</p>
Air pressure	700 to 1300 hPa
Humidity	10 to 90 % (to 95 % briefly) relative humidity
Device data	
Protection class	IP 67 for devices with sensors
Alarm volume	Typically 90 dB (A) in 30 cm distance
Operation time	
– Alkaline battery	Typically 12 hours under normal conditions
– NiMH power pack:	
T4 (HBT 0000)	Typically 12 hours under normal conditions
T4 HC (HBT 0100)	Typically 13 hours under normal conditions
Dimensions	approx. 130 mm x 48 mm x 44 mm (H x W x D)
Weight	approx. 220 g to 250 g
Storage time	
X-am 5000	1 year
Sensors	1 year
Position of use	any
Refresh interval for display and signals	1 s

1) Not part of the BVS 10 ATEX E 080 X and PFG 10 G 001 X technical suitability tests.

Order List

Name and description	Order no.
<p>Dräger X-am 5000</p> <p>Unlimited multi gas detector for 1 to 5 gases with replaceable sensors. With selectable special calibration. Default calibration for the ex-sensor: methane. With default alarm thresholds that can be adjusted specifically for each country.</p>	<p>83 20 000</p>
<p>Power supply units:</p> <p>NiMH power pack T4 83 18 704</p> <p>NiMH power pack HBT 0100 T4 HC 83 22 244</p> <p>Battery holder ABT 0100¹⁾ (without alkaline batteries) 83 22 237</p> <p>Alkaline batteries T3 (2x)¹⁾ 83 22 239</p> <p>Alkaline batteries T4 (2x)¹⁾ 83 22 240</p> <p>Battery and charger set (includes NiMH power pack T4, charger module for Dräger X-am 1/2/5000 and plug-in power supply unit) 83 18 785</p> <p>HC battery and charger set (includes NiMH power pack HBT 0100 T4 HC, charger module for Dräger X-am 1/2/5000 and plug-in power supply unit) 83 22 785</p>	
<p>Chargers:</p> <p>Charging adapter for Dräger X-am 1/2/5000 83 26 101</p> <p>Charger module for Dräger X-am 1/2/5000 83 18 639</p> <p>Power supply unit with cable (worldwide) for max. 20 Dräger X-am 1/2/5000 charger modules 83 15 805</p> <p>Plug-in power supply unit (worldwide) for max. 5 Dräger X-am 1/2/5000 charger modules 83 16 994</p> <p>Plug-in power supply unit (worldwide) for max. 2 Dräger X-am 1/2/5000 charger modules 83 15 635</p> <p>Vehicle connection, 12 V/24 V for Dräger X-am 1/2/5000 charger module 45 30 057</p> <p>Vehicle mount for 1 Dräger X-am 1/2/5000 charger module 83 18 779</p>	

Name and description	Order no.
<p>Accessories</p> <p>The accessories are not part of BVS10 ATEX E 080X and PFG 10 G 001X.</p>	
<p>Pump accessories:</p> <p>Dräger Pump X-am 1/2/5000</p> <p>Case for Dräger Pump X-am 1/2/5000</p> <p>Dräger X-am Pump</p> <p>Case for Dräger X-am Pump</p> <p>USB power supply unit (for Dräger X-am Pump)</p> <p>USB cable (for Dräger X-am Pump)</p> <p>Rubber ball pump</p> <p>Manual pump adapter</p> <p>Filter set for X-am 1/2/5000</p>	<p>83 19 400</p> <p>83 19 385</p> <p>83 27 100</p> <p>83 27 104</p> <p>83 27 102</p> <p>83 24 992</p> <p>68 01 933</p> <p>83 19 195</p> <p>83 19 364</p>
<p>Extension hoses and probes (excerpt):</p> <p>Measuring probe²⁾, 0.5 m</p> <p>Measuring probe²⁾, 1.5 m</p> <p>Telescopic probe²⁾, plug-in</p> <p>Telescopic probe²⁾ 100 with accessories</p> <p>Telescopic probe²⁾ 150 stainless steel</p> <p>Bar probe²⁾ 90</p> <p>Floating probe with accessories (transparent)</p> <p>Fluoroelastomer hose (5 mm), sold by the metre, specify length when ordering</p> <p>Hose CR-NR (rubber, 5 mm), sold by the metre, specify length when ordering</p> <p>3 mm tube connection set³⁾</p> <p>5 mm tube connection set</p> <p>Floating probe (3 mm), EPP, 3 m hose³⁾</p> <p>Floating probe (3 mm), EPP, 10 m hose³⁾</p>	<p>64 08 238</p> <p>64 08 239</p> <p>68 01 954</p> <p>83 16 530</p> <p>83 16 533</p> <p>83 16 532</p> <p>83 18 371</p> <p>12 03 150</p> <p>11 80 681</p> <p>83 27 641</p> <p>83 27 642</p> <p>83 25 831</p> <p>83 25 832</p>

Name and description	Order no.
Fluoroelastomer hose (3 mm) incl. adapter, 5 m ³)	83 25 705
Fluoroelastomer hose (3 mm) incl. adapter, 10 m ³)	83 25 706
Fluoroelastomer hose (3 mm) incl. adapter, 20 m ³)	83 25 707
Fluoroelastomer hose ⁴⁾ (3 mm), sold by the metre, specify length when ordering	83 25 837
Hose (3 mm) ⁴⁾ , PVC, sold by the metre, specify length when ordering	83 25 838
Hose (rubber, 3 mm) ⁴⁾ , CR-NR, sold by the metre, specify length when ordering	83 25 839
Accessories for recording the measured values and for configuration: Dräger GasVision (trial version available at www.draeger.com/software) Dräger GasVision licence key (full version) Dräger CC-Vision (full version available at www.draeger.com/software) USB DIRA with USB cable (USB infrared adapter for communication between Dräger X-am 1/2/5000 and PC)	83 25 646 83 17 409
Calibration accessories: Dräger X-dock, e.g. X-dock 5300 X-am 125 Bump test station, incl. mixed-gas cylinder Calibration cradle for Dräger X-am 1/2/5000 Mixed-gas cylinder 2.5 vol.% CH ₄ , 18 vol.% O ₂ , 15 ppm H ₂ S, 50 ppm CO Test gas cylinder, propane, 0.9 vol.% C ₃ H ₈ in air On-demand controller Standard controller	83 21 880 83 19 130 83 18 752 68 11 130 68 11 118 83 16 556 68 10 397
Other accessories: Protective sleeve for Dräger X-am 1/2/5X00 Carrying bag	83 21 506 83 18 755

Name and description	Order no.
Spare parts	
DrägerSensor CatEx 125 PR, 0 to 100 %LEL (or 0 to 100 vol.% methane)	68 12 950
DrägerSensor Cat Ex 125 PR Gas, 0 to 100 %LEL	68 13 080
DrägerSensor XXS O ₂ , 0 to 25 vol.% ⁵⁾	68 10 881
DrägerSensor XXS O ₂ 100, 0 to 100 vol.%	68 12 385
DrägerSensor XXS CO, 0 to 2000 ppm ¹⁾	68 10 882
DrägerSensor XXS H ₂ S, 0 to 200 ppm ¹⁾	68 10 883
DrägerSensor XXS CO LC, 0 to 2000 ppm ¹⁾	68 13 210
Other DrägerSensors	upon request ⁶⁾

- 1) Not part of the BVS10 ATEX E 080X and PFG 10 G 001X technical suitability test.
- 2) The filter set for X-am 1/2/5000 (order no. 83 19 364) includes a 5 mm tube connection set to connect the probe to the pump.
- 3) This accessory is optimised for the Dräger X-am Pump (market launch in 2017) (for hoses with 3 mm inner diameter).
- 4) 3 mm tube connection set (order no. 83 27 641) required.
- 5) Expected sensor life time: O₂, CO and H₂S >5 years, CatEx > 3 years.
- 6) Data sheets for all sensors that may be used with the device can be downloaded from the product page of the X-am 5000 on the following website: www.draeger.com.

Dräger Safety AG & Co. KGaA

Revalstraße 1

D-23560 Lübeck

Germany

Phone +49 451 8 82- 0

Fax +49 451 8 82- 20 80

www.draeger.com

90 23 999 - TM 4638.210 en

© Dräger Safety AG & Co. KGaA

Edition 16 - January 2018

(Edition 01 - April 2007)

Subject to alteration